

POWDER SLUSH COLD OIL RETURN

Customer: PTRHTF30023

INOAC INTERIOR SYSTEMS 575 JAMES STREET SOUTH ST MARYS, ON N4X 1B9 CA

Attn: Brent Dietrich Tel: (519)808-0372

E-Mail: bdietrich@inoacusa.com

System Information

System Volume: 14000 ltr

Bulk Operating Temp: 500F / 260C

Heating Source:

Blanket:

Fluid: PETRO CANADA CALFLO LT

Make: BP&R CONSTRUCTION

Sample Information

Lab No: 02568915 Analyst: Yen Garcia Sample Date: 07/07/23 Received Date: 07/10/23 Completed: 08/22/23


Yen Garcia


yen.garcia@HFSinclair.com

Recommendation: All the oil parameters are within specs. Continue monitoring.


Comments:

Sample Date	Received Date	Fluid Age	Sample Location	Flash Point (COC)	Water (KF)	Viscosity (40°C)	Acid Number	Solids	GCD 10%	GCD 50%	GCD 90%	GCD % < 335°C
	mm/dd/yy			°F/°C	ppm	cSt	mg/KOH/ g	%wt	°F/°C	°F/°C	°F/°C	%
07/07/23	07/10/23	0.0h	RETURN	331 / 166	27.1	7	0.15	0.039	606 / 319	636 / 336	741 / 394	47.53
12/23/22	01/05/23	0.0h	COLD OIL RETURN	327 / 164	9.0	7.1	0.16	0.109	609 / 321	638 / 337	742 / 394	45.45
08/02/22	08/08/22	0.0h		360 / 182	25.8	7.1	0.20	0.217	607 / 319	636 / 335	739 / 393	48.33
12/24/21	01/07/22	0.0h		338 / 170	8.5	7.1	0.16	0.026	606 / 319	636 / 335	738 / 392	48.62
07/22/21	07/23/21	0.0h		360 / 182	24.5	7.1	0.15	0.146	606 / 319	635 / 335	735 / 391	49.73
Baseline Data				349 / 176		7.52	0.1		604 / 318	640 / 338	734 / 390	47.0

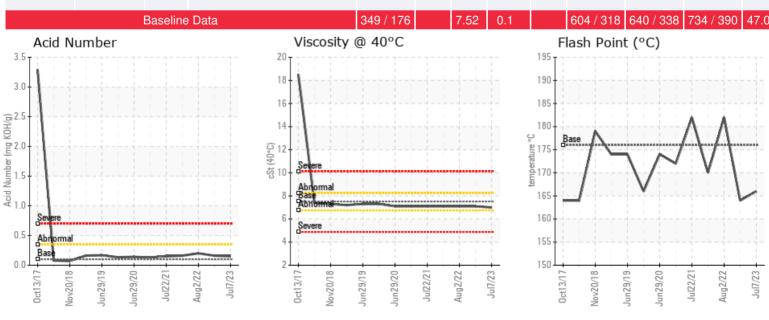

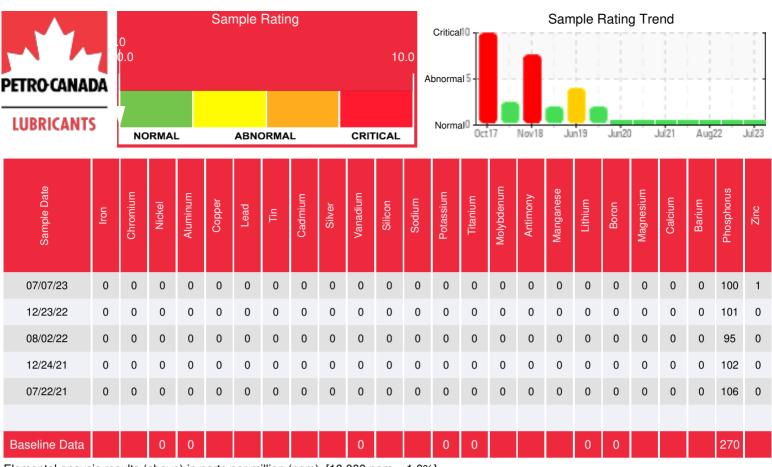

Elemental analysis results (above) in parts per million (ppm). [10,000 ppm = 1.0%]

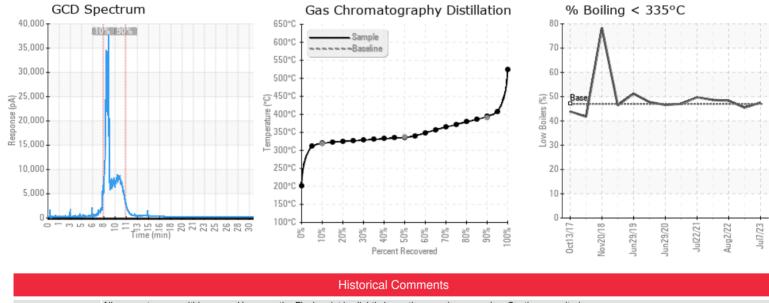

Historical Comments						
12/23/22	All parameters are within specs. However, the Flash point is slightly lower than previous samples. Continue monitoring.					
08/02/22	No action needed at this time.					
12/24/21	Sample results indicate that the fluid is suitable for continue use. Please, sample at the next appropriate interval (6 to 9 months). No action needed at this time.					
07/22/21	Results of the heat transfer oil for the Cold Oil Return are typical for Calflo LT. No evidence of product degradation. Viscosity, Total Acid Number, GCD, Flash Point are within typical parameters. Fluid is suitable for continued use. Submit sample at next appropriate interval (6 - 9 months).					

Petro-Canada makes no representation or warranty of any kind, either express or implied, as to the accuracy or completeness of the analysis and assumes no responsibility and shall have no liability whatsoever with respect to such analysis, or a party's use of it. Petro-Canada is a division of HollyFrontier Corporation.