




**2787 - 0803202001AB**



| Customer:   | System Information  | Sample Information  |
|---|---|---|
| SAINT-GOBAIN PERFORMANCE PLASTICS<br>701 DANIEL WEBSTER HWY<br>MERRIMACK, NH 03054 USA<br>Attn: NORMAN LACHANCE<br>Tel: (603)420-1494<br>E-Mail: norman.r.lachance@saint- | System Volume: 0 gal<br>Bulk Operating Temp: Not Specified<br>Heating Source:<br>Blanket:<br>Fluid: MOBIL MOBILTHERM 603<br>Make: | Lab No: 05601781<br>Analyst: Doug Bogart<br>Sample Date: 06/01/22<br>Received Date: 07/27/22<br>Completed: 08/02/22<br>Doug Bogart<br>doug@wearcheckusa.com |

Recommendation: No corrective action is recommended at this time. Resample at the next service interval to monitor.

Comments: All component wear rates are normal. Moderate concentration of visible dirt/debris present in the fluid. The water content is negligible. The AN level is acceptable for this fluid. The condition of the fluid is suitable for further service.

| Sample Date   | Received Date | Fluid Age | Sample Location | Flash Point (COC) | Water (KF) | Viscosity (40°C) | Acid Number | Solids | GCD 10% | GCD 50% | GCD 90% | GCD % < 335°C |
|---------------|---------------|-----------|-----------------|-------------------|------------|------------------|-------------|--------|---------|---------|---------|---------------|
|               | mm/dd/yy      |           |                 | °F/°C             | ppm        | cSt              | mg/KOH/g    | %wt    | °F/°C   | °F/°C   | °F/°C   | %             |
| 06/01/22      | 07/27/22      | 0.0h      |                 | 390 / 199         | 750        | 20.8             | 0.071       |        |         |         |         |               |
| 02/11/21      | 02/12/21      | 0.0h      | POSTPAID        | 415 / 213         | 2140       | 21.00            | 0.067       |        |         |         |         |               |
| Baseline Data |               |           |                 | 379 / 193         |            | 20.2             | 0.03        |        |         |         |         |               |

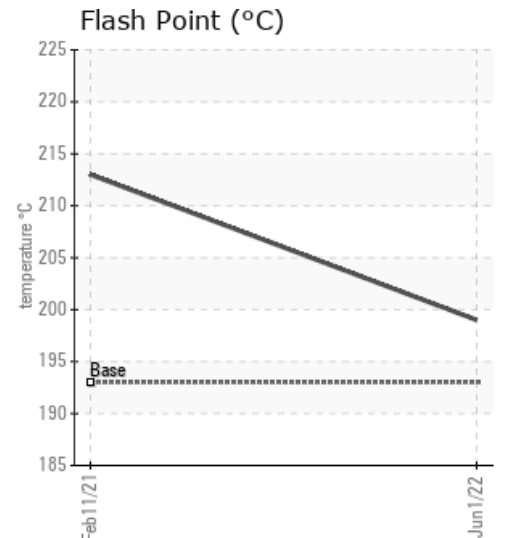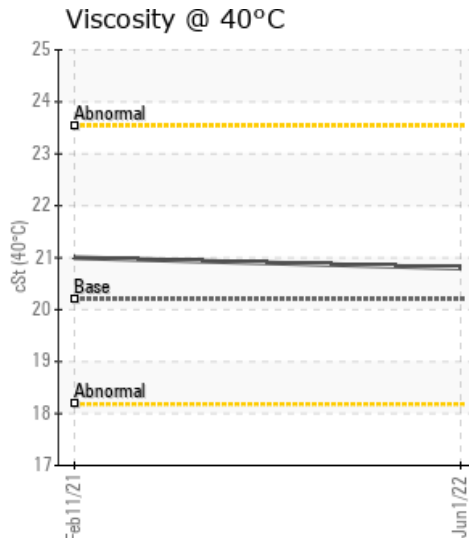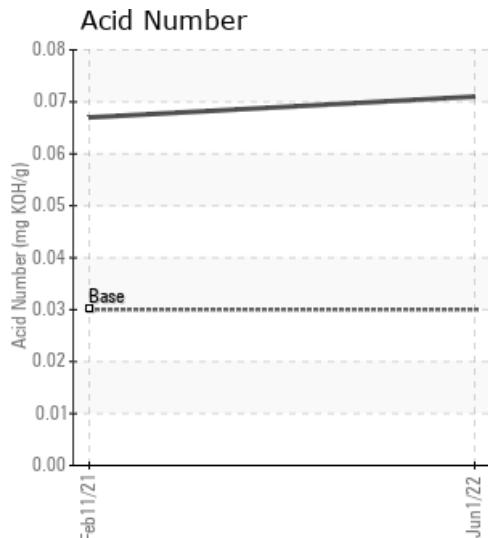

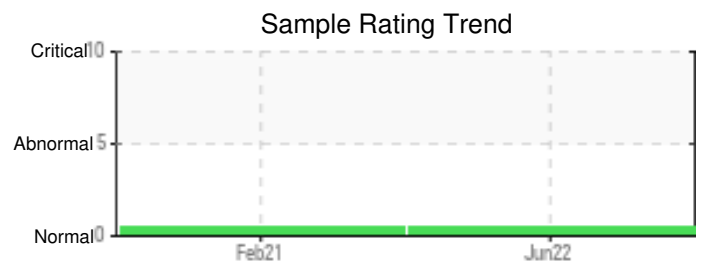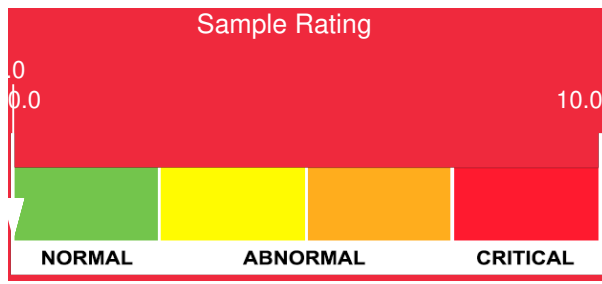

| Sample Date   | Iron | Chromium | Nickel | Aluminum | Copper | Lead | Tin | Cadmium | Silver | Vanadium | Silicon | Sodium | Potassium | Titanium | Molybdenum | Antimony | Manganese | Lithium | Boron | Magnesium | Calcium | Barium | Phosphorus | Zinc |
|---------------|------|----------|--------|----------|--------|------|-----|---------|--------|----------|---------|--------|-----------|----------|------------|----------|-----------|---------|-------|-----------|---------|--------|------------|------|
| 06/01/22      | 6    | 0        | 0      | 0        | 0      | 0    | 2   | 0       | 0      | 0        | 0       | 0      | 0         | 0        | 0          | 0        | 0         | 0       | 0     | 0         | 0       | 0      | 12         | 0    |
| 02/11/21      | 20   | 0        | 0      | 0        | 0      | 0    | 0   | 0       | 0      | 0        | 0       | 0      | 0         | 0        | 0          | 0        | 0         | 0       | 0     | 0         | 0       | 0      | 1          | 0    |
| Baseline Data |      |          | 0      | 0        |        |      |     |         |        | 0        |         |        | 0         | 0        |            |          |           |         | 0     |           |         |        | 0          |      |

Elemental analysis results (above) in parts per million (ppm). [10,000 ppm = 1.0%]

GCD Spectrum

**Historical Comments**

|          |   |
|----------|---|
| 02/11/21 | This is a baseline read-out on the submitted sample. There is a light concentration of water present in the fluid. Moderate concentration of visible dirt/debris present in the fluid. The AN level is acceptable for this fluid. |
|          |   |
|          |   |
|          |   |
|          |   |

WearCheck Canada makes no representation or warranty of any kind, either express or implied, as to the accuracy or completeness of the analysis and assumes no responsibility and shall have no liability whatsoever with respect to such analysis, or a party's use of it.