


PROBLEM SUMMARY

Area **1460** Machine Id **1460-5666-4001 - HG NI THICKENER MECH HPU** Component

Hydraulic System

PETRO CANADA HYDREX MV 36 (100 LTR)

COMPONENT CONDITION SUMMARY

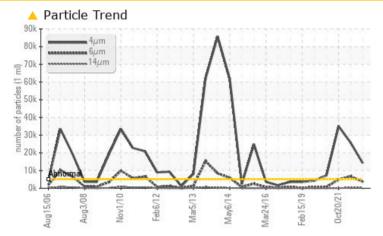

RECOMMENDATION

We advise that you perform a filter service, and use off-line filtration to improve the cleanliness of the system fluid. We recommend an early resample to monitor this condition.

PROBLEMATIC TEST RESULTS							
Sample Status		ABNORMAL	ABNORMAL	ABNORMAL			
Particles >4µm	ASTM D7647 >5000	<u> </u>	<u> </u>	A 35120			
Particles >6µm	ASTM D7647 >1300	A 3761	6 713	4933			
Particles >14µm	ASTM D7647 >160	<u> </u>	<u> </u>	71			
Particles >21µm	ASTM D7647 >40	🔺 139	<u> </u>	17			
Oil Cleanliness	ISO 4406 (c) >19/17	/14 🔺 21/19/16	A 22/20/16	A 22/19/13			


Customer Id: INCVOS Sample No.: PC0057970 Lab Number: 02568902 Test Package: IND 2



To manage this report scan the QR code

To discuss the diagnosis or test data: Kevin Marson +1 (289)291-4644 x4644 Kevin.Marson@wearcheck.com

To change component or sample information: Gloria Gonzalez +1 (289)291-4643 x4643 <u>gloria.gonzalez@wearcheck.com</u>

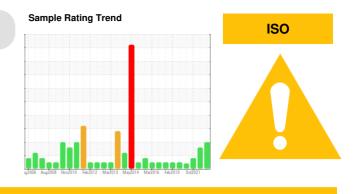

RECOMMENDED ACTIONS						
Action	Status	Date	Done By	Description		
Change Filter			?	We advise that you perform a filter service, and use off-line filtration to improve the cleanliness of the system fluid.		
Resample			?	We recommend an early resample to monitor this condition.		
Filter Fluid			?	We advise that you perform a filter service, and use off-line filtration to improve the cleanliness of the system fluid.		

HISTORICAL DIAGNOSIS



10 Jan 2022 Diag: Kevin Marson

We recommend you service the filters on this component. We recommend an early resample to monitor this condition.All component wear rates are normal. Particles >14µm are abnormally high. Particles >4µm are abnormally high. Particles >6µm are abnormally high. Particles >21µm are notably high. The AN level is acceptable for this fluid. The condition of the oil is suitable for further service.



view report

20 Oct 2021 Diag: Wes Davis

We recommend you service the filters on this component. We recommend an early resample to monitor this condition.All component wear rates are normal. Particles >4µm are abnormally high. Particles >6µm are abnormally high. The AN level is acceptable for this fluid. The condition of the oil is suitable for further service.



24 Jul 2020 Diag: Wes Davis

We recommend you service the filters on this component. Resample at the next service interval to monitor.All component wear rates are normal. There is a light amount of silt (particulates < 14 microns in size) present in the oil. The AN level is acceptable for this fluid. The condition of the oil is suitable for further service.





OIL ANALYSIS REPORT

Area **1460** 1460-5666-4001 - HG Ni THICKEN Component

Hydraulic System

PETRO CANADA HYDREX MV 36 (100 LTR)

DIAGNOSIS

Recommendation

We advise that you perform a filter service, and use off-line filtration to improve the cleanliness of the system fluid. We recommend an early resample to monitor this condition.

Wear

All component wear rates are normal.

Contamination

There is a moderate amount of particulates (2 to 100 microns in size) present in the oil.

Fluid Condition

The AN level is acceptable for this fluid. The oil is still serviceable provided that the contaminant(s) can be reduced to acceptable levels.

SIS REPO	DRT				100000	ISO
ENER MECH	HDII					
R)						
		1g2006 Aug201	08 Nov2010 Feb2012 Ma	r2013 May2014 Mar2016 Feb2019	0ct2021	
SAMPLE INFOR		method	limit/base		history 1	history 2
Sample Number		Client Info		PC0057970	PC0039890	PC0030023
Sample Date		Client Info		25 Jun 2023	10 Jan 2022	20 Oct 2021
Machine Age	mths	Client Info		0	0	0
Oil Age	mths	Client Info		0	0	0
Oil Changed		Client Info		N/A	N/A	N/A
Sample Status				ABNORMAL	ABNORMAL	ABNORMAL
WEAR METAL	S	method	limit/base	current	history 1	history 2
PQ		ASTM D8184*		0		
Iron	ppm	ASTM D5185(m)	>20	<1	<1	1
Chromium	ppm	ASTM D5185(m)	>20	0	0	0
Nickel	ppm	ASTM D5185(m)	>20	<1	<1	<1
Titanium	ppm	ASTM D5185(m)		0	0	0
Silver	ppm	ASTM D5185(m)		0	0	0
Aluminum	ppm	ASTM D5185(m)	>20	0	<1	<1
Lead	ppm	ASTM D5185(m)		0	<1	<1
Copper	ppm	ASTM D5185(m)	>20	<1	<1	<1
Tin	ppm	ASTM D5185(m)	>20	0	0	0
Antimony	ppm	ASTM D5185(m)		0	0	<1
Vanadium Beryllium	ppm	ASTM D5185(m) ASTM D5185(m)		0	0	0
Cadmium	ppm ppm	ASTM D5185(m)		0	0	0
	ppm	. ,		-		-
ADDITIVES		method	limit/base	current	history 1	history 2
Boron	ppm	ASTM D5185(m)	0	<1	<1	<1
Barium	ppm	ASTM D5185(m)		0	0	0
Molybdenum	ppm	ASTM D5185(m)		0	0	0
Manganese	ppm	ASTM D5185(m)		0	0	0
Magnesium	ppm	ASTM D5185(m)	0	<1	<1	<1
Calcium	ppm	ASTM D5185(m)		60 222	117	110 288
Phosphorus	ppm	ASTM D5185(m)	236	333	268	
Zinc Sulfur	ppm	ASTM D5185(m) ASTM D5185(m)	317 561	394 881	345 635	359 650
Lithium	ppm ppm	ASTM D5185(m) ASTM D5185(m)	100	<1	<1	<1
CONTAMINAN		method	limit/base		history 1	history 2
Silicon	ppm	ASTM D5185(m)	>15	<1	0	<1
Sodium	ppm	ASTM D5185(m)	. 20	0	0	0
Potassium	ppm	ASTM D5185(m)	>20	0	<1	<1
FLUID CLEAN	LINESS	method	limit/base	current	history 1	history 2
Particles >4µm		ASTM D7647	>5000	14261	2 5768	4 35120
Particles >6µm		ASTM D7647	>1300	<u> </u>	6 713	4 933
Particles >14µm		ASTM D7647	>160	423	4 22	71
Particles >21µm		ASTM D7647		<u> </u>	<u>∧</u> 79	17
Particles >38µm		ASTM D7647	>10	10	7	2
Particles >71µm		ASTM D7647		1	0	0
Oil Cleanliness		ISO 4406 (c)	>19/17/14	<u> </u>	<u> </u>	<u> </u>

Sample Rating Trend



🔺 Particle Count

🔺 Particle Trend

14

491,520 122,880

Ê 30,720 7 68

> 480 120

> > 30

8

100

40

20

Î 80

of particles 60

number of particles (per 1 1.92

OIL ANALYSIS REPORT

т26	FLUID DEGRAD	OATION	method	limit/base	current	history 1
-24 -22 8	Acid Number (AN)	mg KOH/g	ASTM D974*	0.40	0.46	0.40
+20 40	VISUAL		method	limit/base	current	history 1
+20 4406: 1939 Cleanliness	White Metal	scalar	Visual*	NONE	NONE	NONE
-14 -114	Yellow Metal	scalar	Visual*	NONE	NONE	NONE
12 gg	Precipitate	scalar	Visual*	NONE	NONE	NONE
	Silt	scalar	Visual*	NONE	NONE	NONE
μ 21μ 38μ 71μ	Debris	scalar	Visual*	NONE	VLITE	VLITE
μ 21μ 30μ Γιμ	Sand/Dirt	scalar	Visual*	NONE	NONE	NONE
	Appearance	scalar	Visual*	NORML	NORML	NORML
A	Odor	scalar	Visual*	NORML	NORML	NORML
\wedge	Emulsified Water	scalar	Visual*	>0.05	NEG	NEG
	Free Water	scalar	Visual*		NEG	NEG
1	FLUID PROPE	RTIES	method	limit/base	current	history 1
JAN I	Visc @ 40°C	cSt	ASTM D7279(m)	32.25	33.9	36.2
113 114 113	Visc @ 100°C	cSt	ASTM D7279(m)	6.3	6.3	6.6
Mar5/13 May6/14 Mar24/16 Feb15/19 Oct20/21	Viscosity Index (VI)	Scale	ASTM D2270*	148	138	138
	SAMPLE IMAG	ES	method	limit/base	current	history 1
$\gamma \Lambda$. κ	Color				in su	Jan 11/



history 2

history 2

0.50

NONE

NONE

NONE

NONE

VLITE

NONE

NEG

NEG

37.5


6.6

131

NORML

NORML

history 2

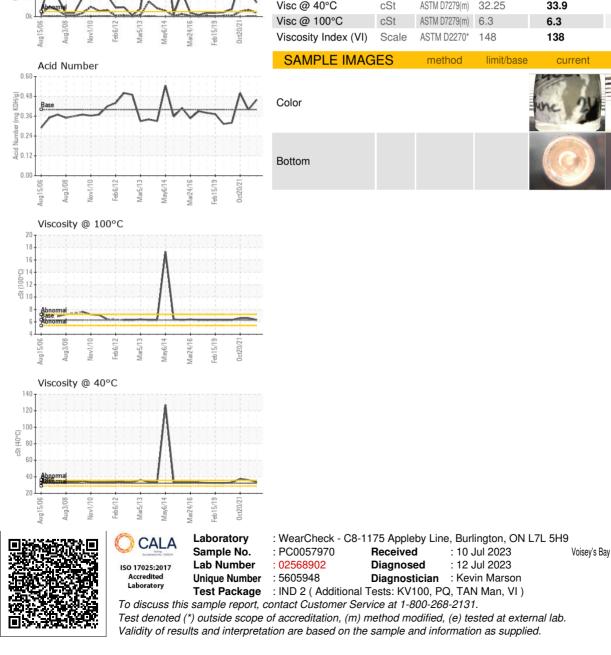

Voisey's Bay Mine Site, P.O. Box 7001, Stn. C Happy Valley Goose Bay, NL CA A0P 1C0 Contact: Robert Feltham robert.feltham@vale.com T: F: x:

Vale - Voisey's Bay