

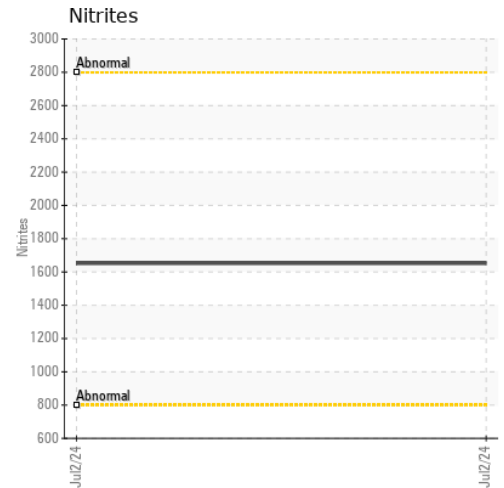
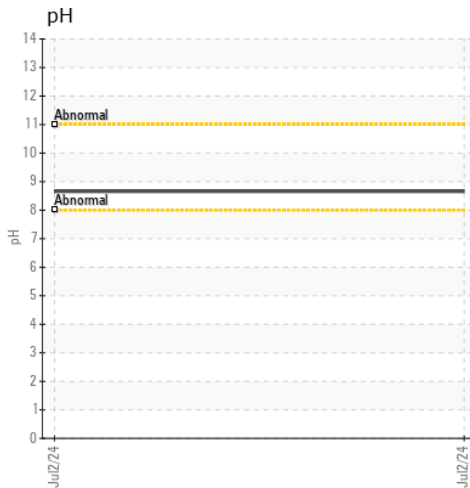
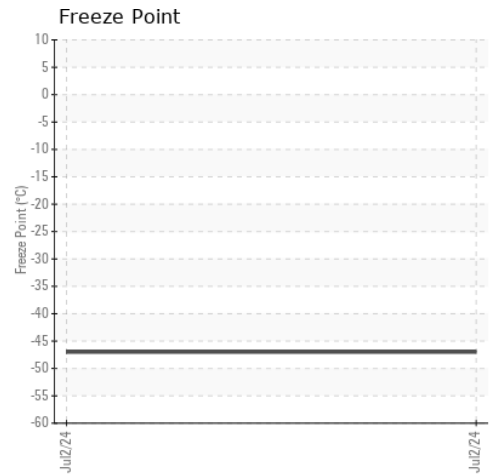
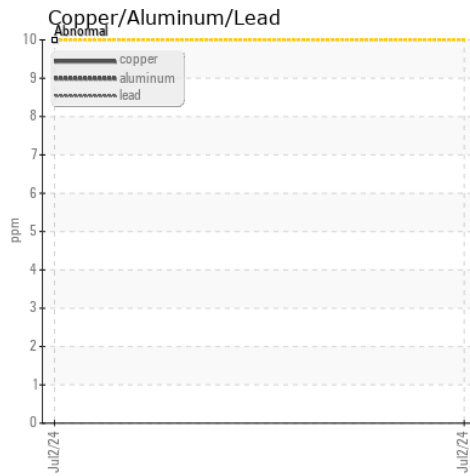
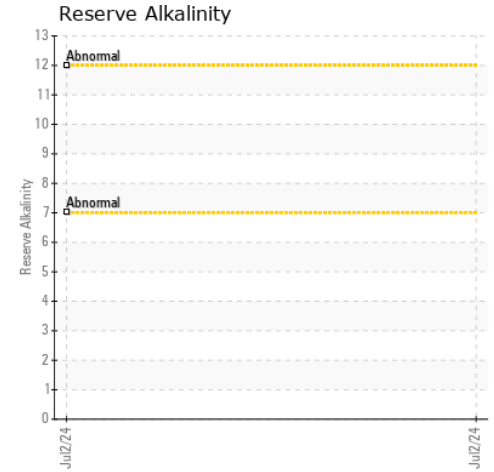


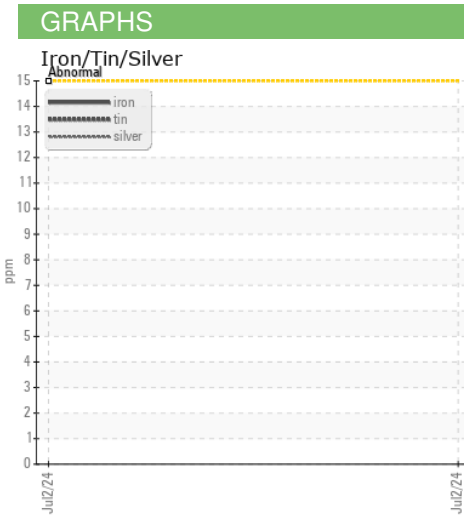

# COOLANT REPORT

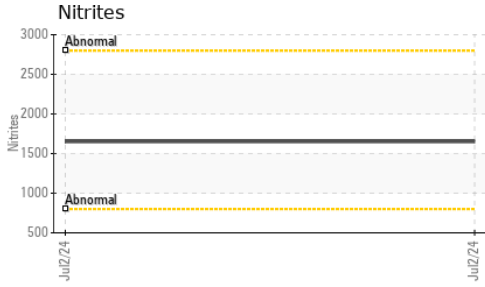

Certificate L2367

**Laboratory** : WearCheck USA - 501 Madison Ave., Cary, NC 27513  
**Sample No.** : PCA0122473  
**Lab Number** : 06230708  
**Unique Number** : 11114201  
**Test Package** : COOL- ( Additional Tests: GlycolType )  
**Received** : 08 Jul 2024  
**Tested** : 10 Jul 2024  
**Diagnosed** : 10 Jul 2024 - Jonathan Hester

To discuss this sample report, contact Customer Service at 1-800-237-1369.

\* - Denotes test methods that are outside of the ISO 17025 scope of accreditation.

Statements of conformity to specifications are based on the simple acceptance decision rule (JCGM 106:2012)

**G LOPES CONSTRUCTION**  
 565 WINTHROP ST  
 TAUNTON, MA  
 US 02780  
 Contact: BUTCH MCGRATH  
 bmcgrath@glopes.com

T:  
F: