




PROBLEM SUMMARY

Sample Rating Trend

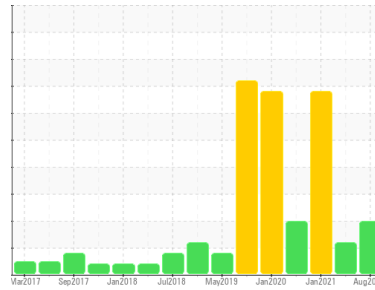


WEAR




Area
Wide Cold Mill/Temper Mill
 Machine Id
80" TEMPER MILL MORGOL (MILL OIL CELLAR) (WCM002) (S/N 100006025)
 Component
Gear Lube System
 Fluid
PETRO CANADA ULTIMA EP 460 (4500 GAL)

COMPONENT CONDITION SUMMARY

▲ Particle Trend

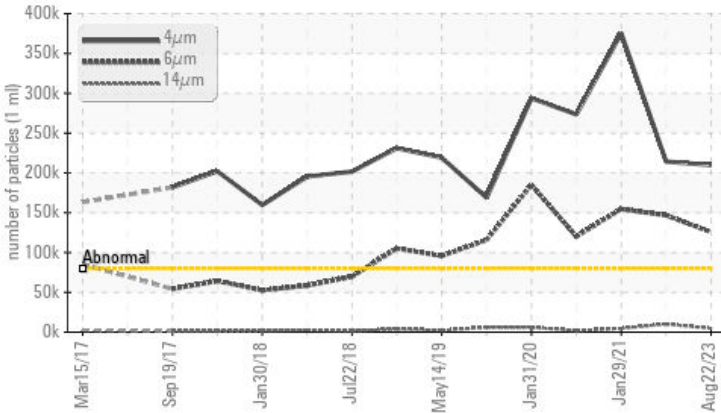

▲ Ferrous Alloys

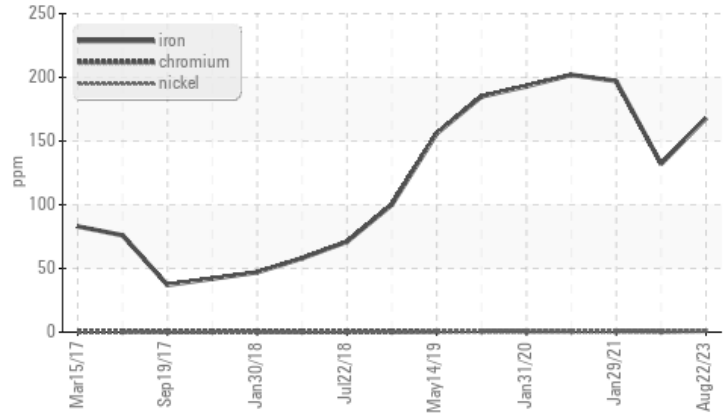

RECOMMENDATION

We recommend you service the filters on this component. We recommend an early resample to monitor this condition. Please contact your representative for information regarding the proper sampling kits for your service. NOTE: We recommend using IND 3 test kits, this testkit includes Analytical Ferrography which provides a detailed morphological analysis of wear particles present in the fluid.

PROBLEMATIC TEST RESULTS

Sample Status			ABNORMAL	ABNORMAL	SEVERE	
Iron	ppm	ASTM D5185(m)	>150	▲ 168	132	▲ 197
Particles >4µm		ASTM D7647	>80000	▲ 209825	▲ 214210	● 375362
Particles >6µm		ASTM D7647	>80000	▲ 125677	▲ 146735	▲ 154654
Oil Cleanliness		ISO 4406 (c)	>23/23/21	▲ 25/24/19	▲ 25/24/20	● 26/24/19

Customer Id: ALGSSM
 Sample No.: WC0752384
 Lab Number: 02577811
 Test Package: IND 2



To manage this report scan the QR code

To discuss the diagnosis or test data:
 Kevin Marson +1 (289)291-4644 x4644
Kevin.Marson@wearcheck.com


To change component or sample information:
 Gloria Gonzalez +1 (289)291-4643 x4643
gloria.gonzalez@wearcheck.com

RECOMMENDED ACTIONS

Action	Status	Date	Done By	Description
Change Filter	---	---	?	We recommend you service the filters on this component.
Resample	---	---	?	We recommend an early resample to monitor this condition.
Contact Required	---	---	?	Please contact your representative for information regarding the proper sampling kits for your service.
Alert	---	---	?	NOTE: We recommend using IND 3 test kits,

HISTORICAL DIAGNOSIS


ISO




01 Mar 2023 Diag: Kevin Marson

We recommend you service the filters on this component. We recommend an early resample to monitor this condition. Please contact your representative for information regarding the proper sampling kits for your service. NOTE: We recommend using IND 3 test kits, this testkit includes Analytical Ferrography which provides a detailed morphological analysis of wear particles present in the fluid. Component wear rates appear to be normal (unconfirmed). Particles >4µm and oil cleanliness are abnormally high. Particles >6µm are notably high. The system cleanliness is above the acceptable limit for the target ISO 4406 cleanliness code. The AN level is acceptable for this fluid. The oil is still serviceable provided that the contaminant(s) can be reduced to acceptable levels.

view report




WATER




29 Jan 2021 Diag: Kevin Marson

We advise that you check for the source of water entry. Check seals and/or filters for points of contaminant entry. We advise that you follow the water drain-off procedure for this component. The air breather requires service. If unrated, we recommend that you replace with a suitable micron rated and/or desiccant air breather. If rated, we recommend that you service/replace the breather. We recommend you service the filters on this component. Resample in 30-45 days to monitor this situation. Please contact your representative for information regarding the proper sampling kits for your service. this testkit includes Analytical Ferrography which provides a detailed morphological analysis of wear particles present in the fluid. Iron ppm levels are marginal. All other component wear rates are normal. Water and ppm water contamination levels are severe. Particles >4µm are severely high. Particles >4µm are severely high.. Particles >4µm are severely high... Particles >6µm are notably high. There is a high concentration of water present in the oil. Free water present. The system cleanliness code is much higher than the acceptable limit for the target ISO 4406 cleanliness code. The AN level is acceptable for this fluid. The oil is still serviceable provided that the contaminant(s) can be reduced to acceptable levels.

view report




WEAR



12 Nov 2020 Diag: Kevin Marson

Check seals and/or filters for points of contaminant entry. The air breather requires service. If unrated, we recommend that you replace with a suitable micron rated and/or desiccant air breather. If rated, we recommend that you service/replace the breather. We recommend you service the filters on this component. Resample in 30-45 days to monitor this situation. Please contact your representative for information regarding the proper sampling kits for your service. NOTE: We recommend using IND 3 test kits, this testkit includes Analytical Ferrography which provides a detailed morphological analysis of wear particles present in the fluid. Iron ppm levels are abnormal. The low ferrous density (PQ) index indicates the wear metal levels are due to corrosion. Particles >4µm are severely high. Particles >6µm are notably high. The system cleanliness code is much higher than the acceptable limit for the target ISO 4406 cleanliness code. The AN level is acceptable for this fluid. The condition of the oil is suitable for further service.


view report





OIL ANALYSIS REPORT

Sample Rating Trend

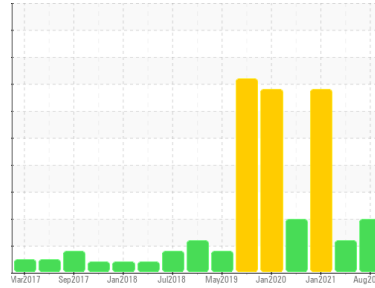

WEAR



Area
Wide Cold Mill/Temper Mill
 Machine Id
80" TEMPER MILL MORGOIL (MILL OIL CELLAR) (WCM002) (S/N 100006025)
 Component
Gear Lube System
 Fluid
PETRO CANADA ULTIMA EP 460 (4500 GAL)

DIAGNOSIS

Recommendation

We recommend you service the filters on this component. We recommend an early resample to monitor this condition. Please contact your representative for information regarding the proper sampling kits for your service. NOTE: We recommend using IND 3 test kits, this testkit includes Analytical Ferrography which provides a detailed morphological analysis of wear particles present in the fluid.

Wear

Iron ppm levels are marginal. All other component wear rates are normal.

Contamination

There is a moderate amount of silt (particulates < 14 microns in size) present in the oil. The system cleanliness is above the acceptable limit for the target ISO 4406 cleanliness code.

Fluid Condition

The AN level is acceptable for this fluid. The oil is still serviceable provided that the contaminant(s) can be reduced to acceptable levels.

SAMPLE INFORMATION

	method	limit/base	current	history1	history2
Sample Number	Client Info		WC0752384	WC0752204	WC0419565
Sample Date	Client Info		22 Aug 2023	01 Mar 2023	29 Jan 2021
Machine Age	hrs	Client Info	0	0	0
Oil Age	hrs	Client Info	0	0	0
Oil Changed	Client Info		N/A	N/A	N/A
Sample Status			ABNORMAL	ABNORMAL	SEVERE

WEAR METALS

	method	limit/base	current	history1	history2
PQ	ASTM D8184*		10	17	---
Iron	ppm	ASTM D5185(m) >150	▲ 168	132	▲ 197
Chromium	ppm	ASTM D5185(m) >10	1	<1	<1
Nickel	ppm	ASTM D5185(m) >10	<1	1	1
Titanium	ppm	ASTM D5185(m)	0	0	0
Silver	ppm	ASTM D5185(m)	0	0	<1
Aluminum	ppm	ASTM D5185(m) >25	1	1	2
Lead	ppm	ASTM D5185(m) >100	<1	<1	0
Copper	ppm	ASTM D5185(m) >50	2	2	4
Tin	ppm	ASTM D5185(m) >10	2	2	4
Antimony	ppm	ASTM D5185(m) >5	0	<1	<1
Vanadium	ppm	ASTM D5185(m)	0	0	0
Beryllium	ppm	ASTM D5185(m)	0	0	0
Cadmium	ppm	ASTM D5185(m)	0	0	0

ADDITIVES

	method	limit/base	current	history1	history2
Boron	ppm	ASTM D5185(m) 111	<1	1	3
Barium	ppm	ASTM D5185(m)	0	0	0
Molybdenum	ppm	ASTM D5185(m) 0	<1	<1	<1
Manganese	ppm	ASTM D5185(m)	1	<1	<1
Magnesium	ppm	ASTM D5185(m) 2	1	<1	1
Calcium	ppm	ASTM D5185(m) 6	5	<1	8
Phosphorus	ppm	ASTM D5185(m) 482	141	185	240
Zinc	ppm	ASTM D5185(m) 3	4	3	3
Sulfur	ppm	ASTM D5185(m) 1458	4366	5224	10872
Lithium	ppm	ASTM D5185(m)	<1	<1	<1

CONTAMINANTS






	method	limit/base	current	history1	history2
Silicon	ppm	ASTM D5185(m) >50	6	5	8
Sodium	ppm	ASTM D5185(m)	3	3	7
Potassium	ppm	ASTM D5185(m) >20	7	8	5

FLUID CLEANLINESS

	method	limit/base	current	history1	history2
Particles >4µm	ASTM D7647	>80000	▲ 209825	▲ 214210	● 375362
Particles >6µm	ASTM D7647	>80000	▲ 125677	▲ 146735	▲ 154654
Particles >14µm	ASTM D7647	>20000	4759	9990	4687
Particles >21µm	ASTM D7647	>5000	437	968	859
Particles >38µm	ASTM D7647	>1300	8	15	52
Particles >71µm	ASTM D7647	>320	3	2	4
Oil Cleanliness	ISO 4406 (c)	>23/23/21	▲ 25/24/19	▲ 25/24/20	● 26/24/19



OIL ANALYSIS REPORT

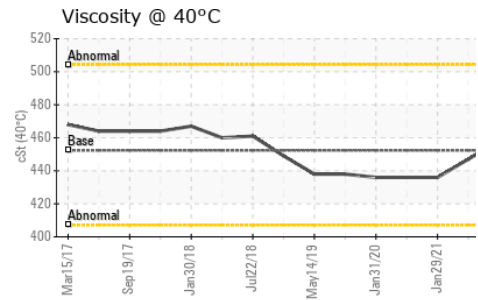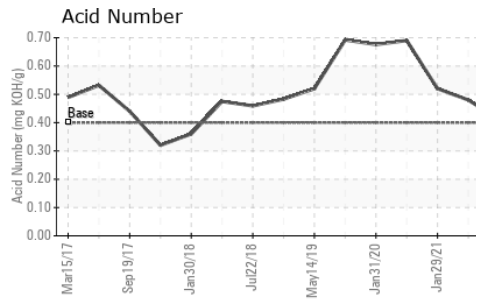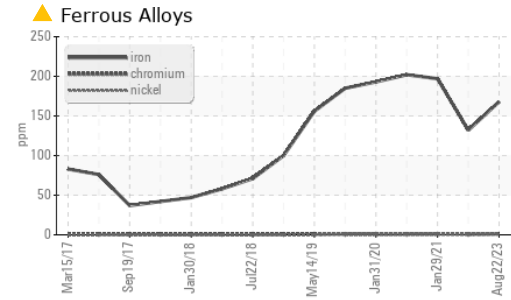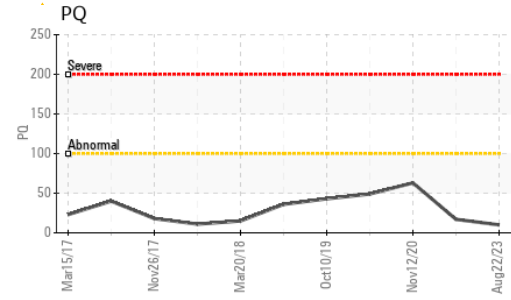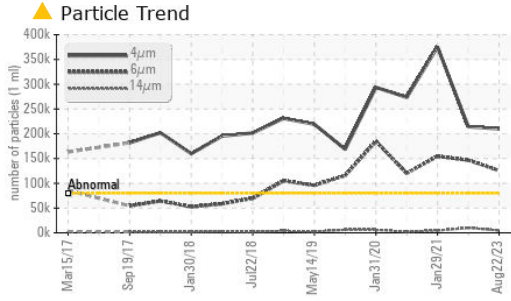






FLUID DEGRADATION	method	limit/base	current	history1	history2	
Acid Number (AN)	mg KOH/g	ASTM D974*	0.4	0.41	0.48	0.52

VISUAL	method	limit/base	current	history1	history2	
White Metal	scalar	Visual*	NONE	NONE	NONE	NONE
Yellow Metal	scalar	Visual*	NONE	NONE	NONE	NONE
Precipitate	scalar	Visual*	NONE	NONE	NONE	NONE
Silt	scalar	Visual*	NONE	NONE	NONE	NONE
Debris	scalar	Visual*	NONE	NONE	NONE	VLITE
Sand/Dirt	scalar	Visual*	NONE	NONE	NONE	NONE
Appearance	scalar	Visual*	NORML	NORML	NORML	NORML
Odor	scalar	Visual*	NORML	NORML	NORML	NORML
Emulsified Water	scalar	Visual*	>0.1	NEG	NEG	▲.5%
Free Water	scalar	Visual*		NEG	NEG	▲.5%

FLUID PROPERTIES	method	limit/base	current	history1	history2	
Visc @ 40°C	cSt	ASTM D7279(m)	452.3	458	447	436

SAMPLE IMAGES	method	limit/base	current	history1	history2
Color					
Bottom					

GRAPHS

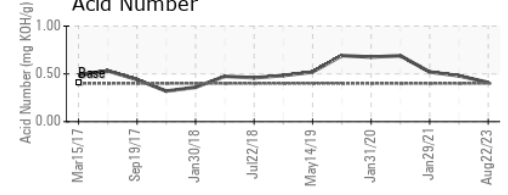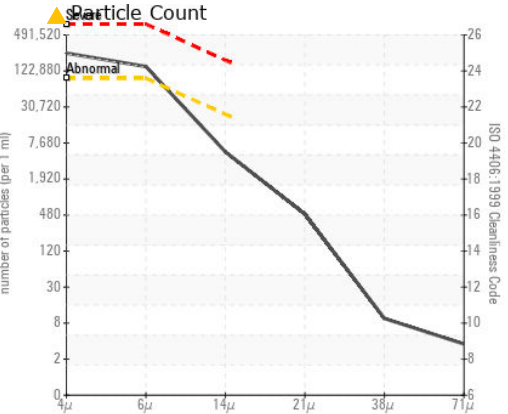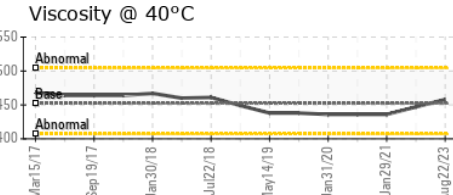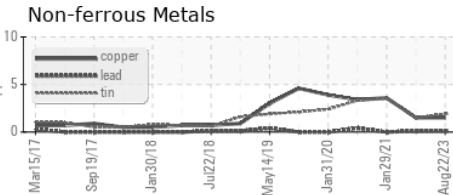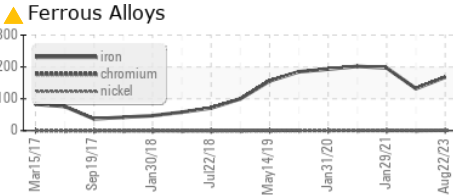

Laboratory : WearCheck - C8-1175 Appleby Line, Burlington, ON L7L 5H9 **ALGOMA STEEL INC. - STORES DEPT.**
Sample No. : WC0752384 **Received** : 23 Aug 2023 301 WALLACE TERRACE
Lab Number : **02577811** **Diagnosed** : 25 Aug 2023 SAULT STE MARIE, ON
Unique Number : 5630871 **Diagnostician** : Kevin Marson CA P6C 1K8
Test Package : IND 2 (Additional Tests: PQ)
 Contact: Algoma Reliability
 algomareliability@algoma.com

To discuss this sample report, contact Customer Service at 1-800-268-2131.
 Test denoted (*) outside scope of accreditation, (m) method modified, (e) tested at external lab.
 Validity of results and interpretation are based on the sample and information as supplied.
 T: (705)206-1059
 F: (705)945-3585