

OIL ANALYSIS REPORT

Chem-Ecol A2308125

Component

Unknown Component

GEAR OIL ISO 150 (--- GAL)

Sample Rating Trend



Recommendation

This is a baseline read-out on the submitted sample.

Wear

{not applicable}

Contamination

{not applicable}


Fluid Condition

Acid Number (AN) is notably high.

				Aug2023		
SAMPLE INFOR	MATION	l method	limit/base	current	history1	history2
Sample Number		Client Info		E3000043		
Sample Date		Client Info		23 Aug 2023		
Machine Age	hrs	Client Info		0		
Oil Age	hrs	Client Info		0		
Oil Changed		Client Info		N/A		
Sample Status				NORMAL		
WEAR METALS		method	limit/base	current	history1	history2
Iron	ppm	ASTM D5185(m)		1		
Chromium	ppm	ASTM D5185(m)		0		
Nickel	ppm	ASTM D5185(m)		<1		
Titanium	ppm	ASTM D5185(m)		0		
Silver	ppm	ASTM D5185(m)		0		
Aluminum	ppm	ASTM D5185(m)		<1		
Lead	ppm	ASTM D5185(m)		0		
Copper	ppm	ASTM D5185(m)		0		
Tin	ppm	ASTM D5185(m)		0		
Antimony	ppm	ASTM D5185(m)		0		
Vanadium	ppm	ASTM D5185(m)		0		
Beryllium	ppm	ASTM D5185(m)		0		
Cadmium	ppm	ASTM D5185(m)		0		
ADDITIVES		method	limit/base	current	history1	history2
Boron	ppm	ASTM D5185(m)	50	<1		
Barium	ppm	ASTM D5185(m)	15	0		
Molybdenum	ppm	ASTM D5185(m)	15	0		
Manganese	ppm	ASTM D5185(m)		0		
Magnesium	ppm	ASTM D5185(m)	50	<1		
Calcium	ppm	ASTM D5185(m)	50	1		
Phosphorus	ppm	ASTM D5185(m)	350	536		
Zinc	ppm	ASTM D5185(m)	100	5		
Sulfur	ppm	ASTM D5185(m)	12500	5047		
Lithium	ppm	ASTM D5185(m)	.2000	<1		
CONTAMINANT		method	limit/base	current	history1	history2
Silicon	ppm	ASTM D5185(m)		1		
Sodium		ASTM D5185(m)		<1		
Potassium	ppm	ASTM D5185(m)	>20	0		
Water	ppm %	ASTM D5163(III) ASTM D6304*	>20			
ppm Water	ppm	ASTM D6304*		0.001 12.7		
			l:: t//			history O
FLUID CLEANLI	NESS	method	limit/base	current	history1	history2
Particles >4µm		ASTM D7647	>5000	108		
Particles >6µm		ASTM D7647	>1300	37		
Particles >14µm		ASTM D7647	>160	6		
Particles >21µm		ASTM D7647	>40	3		
Particles >38µm		ASTM D7647	>10	1		
Particles >71μm		ASTM D7647	>3	1		
Oil Cleanliness		ISO 4406 (c)	>19/17/14	14/12/10		



OIL ANALYSIS REPORT

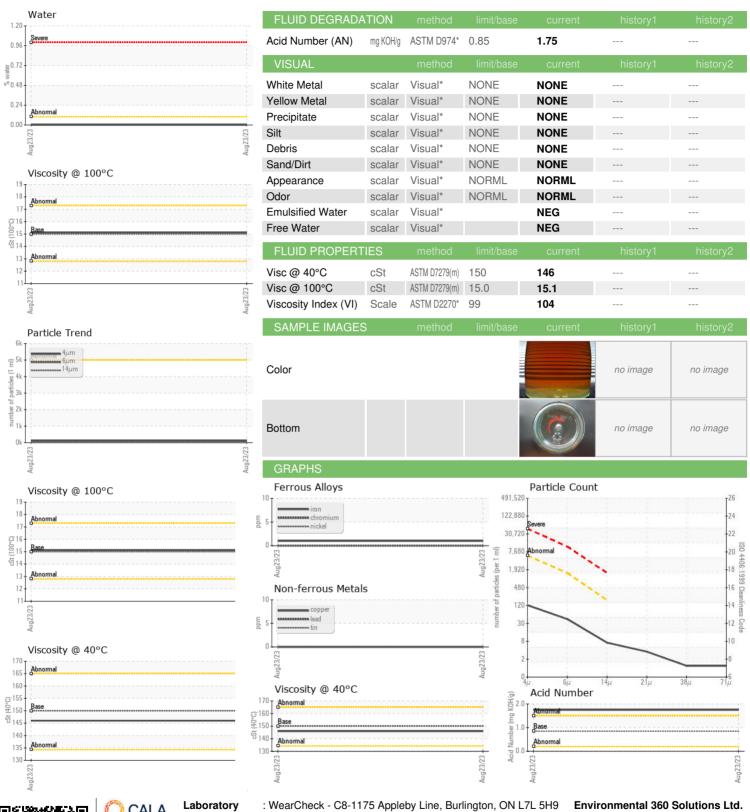



CALA ISO 17025:2017 Accredited

Laboratory

Sample No. Lab Number **Unique Number**

: E30000043

: 02578553

Received Diagnosed : 5631613

: 25 Aug 2023 : 30 Aug 2023

Diagnostician : Tatiana Sorkina

Test Package : IND 2 (Additional Tests: KF, KV100, PrtCount, TAN Man, VI)

To discuss this sample report, contact Customer Service at 1-800-268-2131. Test denoted (*) outside scope of accreditation, (m) method modified, (e) tested at external lab. Validity of results and interpretation are based on the sample and information as supplied.

640 Victoria Street Cobourg, ON **CA K9A 5H5** Contact: Tatiana Sorkina

tsorkina@e360s.ca T: (800)263-3939 F: (905)373-4950