PROBLEM SUMMARY

Area
Direct Strip Mill/Caster
Machine Id
LHO HYDRAULIC SYSTEM (DSC031) (S/N 1000025534)
Component
Hydraulic System
Fluid
HOUGHTON HOUGHTO-SAFE 620 (4750 LTR)

Sample Rating Trend

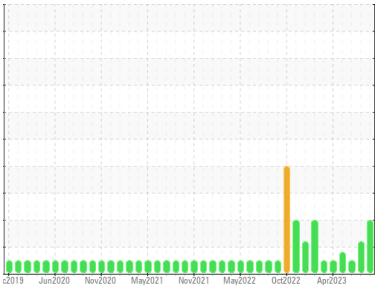

ISO

COMPONENT CONDITION SUMMARY

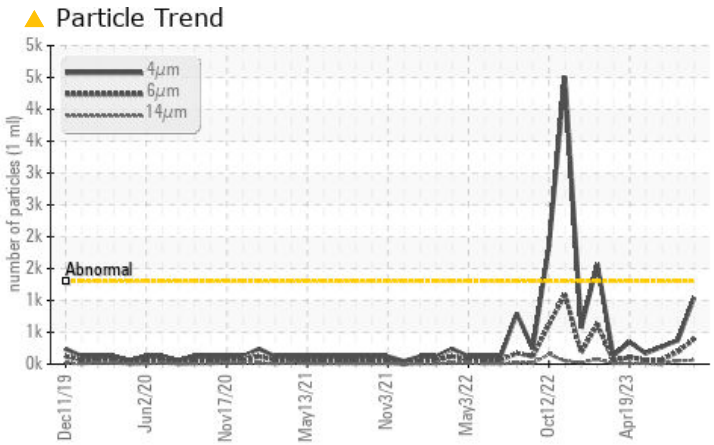

RECOMMENDATION

We advise that you perform a filter service, and use off-line filtration to improve the cleanliness of the system fluid. We recommend an early resample to monitor this condition. Please note that this is a corrected copy for data entry updates.

PROBLEMATIC TEST RESULTS

Sample Status				ABNORMAL	ABNORMAL	NORMAL
Particles >6µm		ASTM D7647	>320	▲ **395**	197	55
Particles >14µm		ASTM D7647	>20	▲ **61**	▲ 53	1
Particles >21µm		ASTM D7647	>4	▲ **25**	▲ 25	3
Particles >38µm		ASTM D7647	>3	▲ **8**	4	2
Oil Cleanliness		ISO 4406 (c)	>17/15/11	▲ **17/16/13**	▲ 16/15/13	15/13/7

Customer Id: ALGSSM
Sample No.: WC0837303
Lab Number: 02586205
Test Package: IND 2

To manage this report scan the QR code

To discuss the diagnosis or test data:
Kevin Marson +1 (289)291-4644 x4644
Kevin.Marson@wearcheck.com

To change component or sample information:
Gloria Gonzalez +1 (289)291-4643 x4643
gloria.gonzalez@wearcheck.com

RECOMMENDED ACTIONS

Action	Status	Date	Done By	Description
Change Filter	---	---	?	We advise that you perform a filter service, and use off-line filtration to improve the cleanliness of the system fluid.
Resample	---	---	?	We recommend an early resample to monitor this condition.
Filter Fluid	---	---	?	We advise that you perform a filter service, and use off-line filtration to improve the cleanliness of the system fluid.

HISTORICAL DIAGNOSIS

09 Aug 2023 Diag: Kevin Marson

ISO

We advise that you perform a filter service, and use off-line filtration to improve the cleanliness of the system fluid. We recommend an early resample to monitor this condition.All component wear rates are normal. There is a moderate amount of particulates (2 to 100 microns in size) present in the oil. The system cleanliness is above the acceptable limit for the target ISO 4406 cleanliness code. The AN level is acceptable for this fluid. The pH level of this fluid is within the acceptable limits. The reserve alkalinity of this fluid is acceptable. The water concentration level is acceptable for this fluid. The oil is still serviceable provided that the contaminant(s) can be reduced to acceptable levels.

view report

22 Jun 2023 Diag: Kevin Marson

NORMAL

Resample at the next service interval to monitor.All component wear rates are normal. The system cleanliness is acceptable for your target ISO 4406 cleanliness code. The system and fluid cleanliness is acceptable. The AN level is acceptable for this fluid. The pH level of this fluid is within the acceptable limits. The reserve alkalinity of this fluid is acceptable. The water concentration level is acceptable for this fluid. The condition of the oil is suitable for further service.

view report

16 May 2023 Diag: Kevin Marson

WEAR

Resample at the next service interval to monitor.Iron ppm levels are noted. All other component wear rates are normal. The system cleanliness is acceptable for your target ISO 4406 cleanliness code. The system and fluid cleanliness is acceptable. The AN level is acceptable for this fluid. The pH level of this fluid is within the acceptable limits. The reserve alkalinity of this fluid is acceptable. The water concentration level is acceptable for this fluid. The condition of the oil is suitable for further service.

view report

OIL ANALYSIS REPORT

Sample Rating Trend

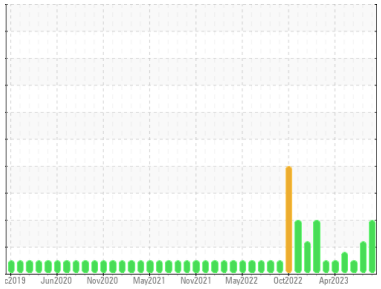

ISO

Area
Direct Strip Mill/Caster
Machine Id
LHO HYDRAULIC SYSTEM (DSC031) (S/N 1000025534)
Component
Hydraulic System
Fluid
HOUGHTON HOUGHTO-SAFE 620 (4750 LTR)

DIAGNOSIS

Recommendation

We advise that you perform a filter service, and use off-line filtration to improve the cleanliness of the system fluid. We recommend an early resample to monitor this condition. Please note that this is a corrected copy for data entry updates.

Wear

All component wear rates are normal.

Contamination

There is a moderate amount of particulates (2 to 100 microns in size) present in the oil. The system cleanliness is above the acceptable limit for the target ISO 4406 cleanliness code.

Fluid Condition

The AN level is acceptable for this fluid. The pH level of this fluid is within the acceptable limits. The reserve alkalinity of this fluid is acceptable. The water concentration level is acceptable for this fluid. The oil is still serviceable provided that the contaminant(s) can be reduced to acceptable levels.

SAMPLE INFORMATION		method	limit/base	current	history1	history2
Sample Number		Client Info		**WC0837303**	WC0813755	WC0780828
Sample Date		Client Info		**27 Sep 2023**	09 Aug 2023	22 Jun 2023
Machine Age	hrs	Client Info		**0**	0	0
Oil Age	hrs	Client Info		**0**	0	0
Oil Changed		Client Info		**N/A**	N/A	N/A
Sample Status				**ABNORMAL**	ABNORMAL	NORMAL

WEAR METALS		method	limit/base	current	history1	history2
Iron	ppm	ASTM D5185(m)	>20	**0**	0	<1
Chromium	ppm	ASTM D5185(m)	>20	**0**	0	<1
Nickel	ppm	ASTM D5185(m)	>20	**0**	0	0
Titanium	ppm	ASTM D5185(m)		**0**	0	0
Silver	ppm	ASTM D5185(m)		**<1**	<1	0
Aluminum	ppm	ASTM D5185(m)	>20	**0**	0	0
Lead	ppm	ASTM D5185(m)	>20	**0**	0	0
Copper	ppm	ASTM D5185(m)	>20	**0**	0	1
Tin	ppm	ASTM D5185(m)	>20	**0**	0	0
Antimony	ppm	ASTM D5185(m)		**0**	0	0
Vanadium	ppm	ASTM D5185(m)		**0**	0	0
Beryllium	ppm	ASTM D5185(m)		**0**	0	0
Cadmium	ppm	ASTM D5185(m)		**0**	0	0

ADDITIVES		method	limit/base	current	history1	history2
Boron	ppm	ASTM D5185(m)		**0**	2	1
Barium	ppm	ASTM D5185(m)		**<1**	1	0
Molybdenum	ppm	ASTM D5185(m)		**0**	0	<1
Manganese	ppm	ASTM D5185(m)		**0**	0	0
Magnesium	ppm	ASTM D5185(m)		**<1**	2	<1
Calcium	ppm	ASTM D5185(m)		**<1**	1	<1
Phosphorus	ppm	ASTM D5185(m)		**0**	<1	<1
Zinc	ppm	ASTM D5185(m)		**0**	0	0
Sulfur	ppm	ASTM D5185(m)		**39**	51	6
Lithium	ppm	ASTM D5185(m)		**<1**	<1	0

CONTAMINANTS		method	limit/base	current	history1	history2
Silicon	ppm	ASTM D5185(m)	>15	**<1**	0	0
Sodium	ppm	ASTM D5185(m)		**18**	13	27
Potassium	ppm	ASTM D5185(m)	>20	**12**	20	21
Water	%	ASTM D6304*	>43.5	**39.9**	38.9	40.7
ppm Water	ppm	ASTM D6304*	>435000	**399000**	389000	407000

FLUID CLEANLINESS		method	limit/base	current	history1	history2
Particles >4µm		ASTM D7647	>1300	**1041**	373	272
Particles >6µm		ASTM D7647	>320	▲ **395**	197	55
Particles >14µm		ASTM D7647	>20	▲ **61**	▲ 53	1
Particles >21µm		ASTM D7647	>4	▲ **25**	▲ 25	3
Particles >38µm		ASTM D7647	>3	▲ **8**	4	2
Particles >71µm		ASTM D7647	>3	**2**	2	0
Oil Cleanliness		ISO 4406 (c)	>17/15/11	▲ **17/16/13**	▲ 16/15/13	15/13/7

OIL ANALYSIS REPORT

Particle Count

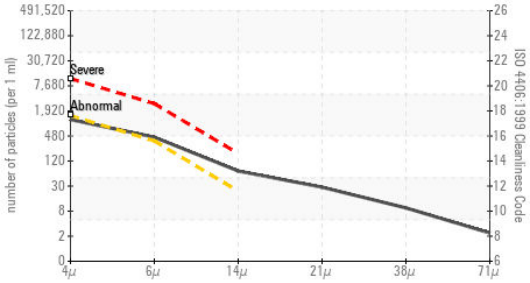

Particle Trend

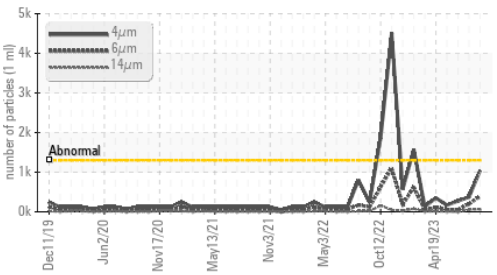

Reserve Alkalinity

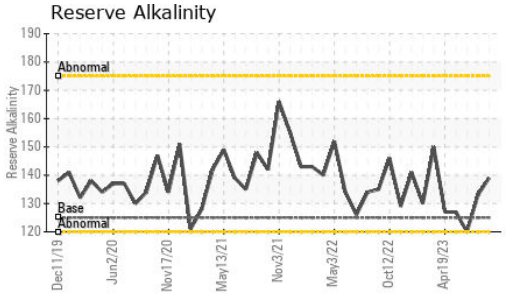

Acid Number

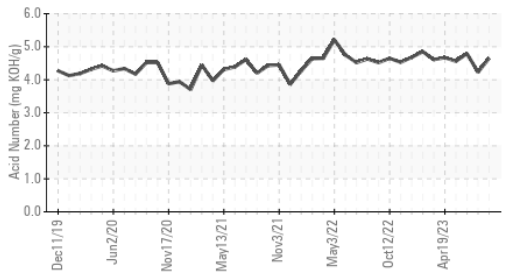

Water (KF)

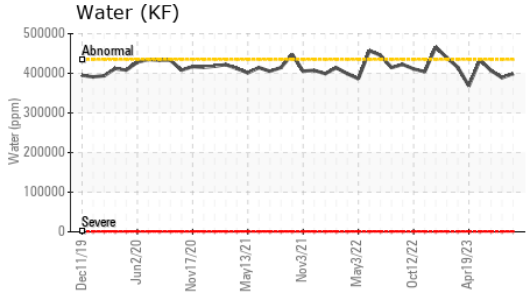

FLUID DEGRADATION		method	limit/base	current	history1	history2
Acid Number (AN)	mg KOH/g	ASTM D974*		**4.65**	4.23	4.79
Alkiline Reserve (Oils)	ml KOH/g	ASTM D1121*	125	**139**	133	120

VISUAL		method	limit/base	current	history1	history2
White Metal	scalar	Visual*	NONE	**NONE**	NONE	NONE
Yellow Metal	scalar	Visual*	NONE	**NONE**	NONE	NONE
Precipitate	scalar	Visual*	NONE	**NONE**	NONE	NONE
Silt	scalar	Visual*	NONE	**NONE**	NONE	NONE
Debris	scalar	Visual*	NONE	**NONE**	NONE	NONE
Sand/Dirt	scalar	Visual*	NONE	**NONE**	NONE	NONE
Appearance	scalar	Visual*	NORML	**FRGLY**	FRGLY	FRGLY
Odor	scalar	Visual*	NORML	**NORML**	NORML	NORML
Emulsified Water	scalar	Visual*	>43.5	**>10%**	>10%	>10%
Free Water	scalar	Visual*		**NEG**	NEG	NEG

FLUID PROPERTIES		method	limit/base	current	history1	history2
pH	Scale 0-14	ASTM D1287*		**9.34**	9.59	9.36
Visc @ 40°C	cSt	ASTM D7279(m)		**42.1**	42.0	42.3

SAMPLE IMAGES	method	limit/base	current	history1	history2
Color					
Bottom					

ISO 17025:2017 Accredited Laboratory

Laboratory : WearCheck - C8-1175 Appleby Line, Burlington, ON L7L 5H9 **ALGOMA STEEL INC. - STORES DEPT.**
Sample No. : WC0837303 **Received** : 02 Oct 2023 301 WALLACE TERRACE
Lab Number : 02586205 **Diagnosed** : 13 Oct 2023 SAULT STE MARIE, ON
Unique Number : 5655271 **Diagnostician** : Kevin Marson CA P6C 1K8
Test Package : IND 2 (Additional Tests: KF, pH, ReserveAlk, TAN Man) Contact: Algoma Reliability

To discuss this sample report, contact Customer Service at 1-800-268-2131. algomareliability@algoma.com
Test denoted (*) outside scope of accreditation, (m) method modified, (e) tested at external lab. T: (705)206-1059
Validity of results and interpretation are based on the sample and information as supplied. F: (705)945-3585