




PROBLEM SUMMARY

Sample Rating Trend


ISO

Area
Direct Strip Mill/Finishing
 Machine Id
PH3 HYDRAULIC SYSTEM (DSC004) (S/N 1000014662)
 Component
Hydraulic System
 Fluid
HOUGHTON HOUGHTO-SAFE 620 (15000 LTR)

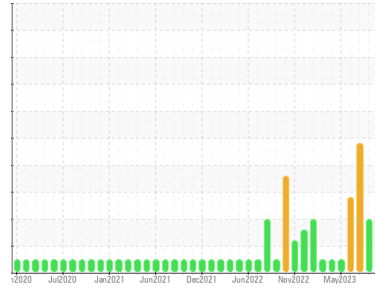

COMPONENT CONDITION SUMMARY

▲ Particle Trend

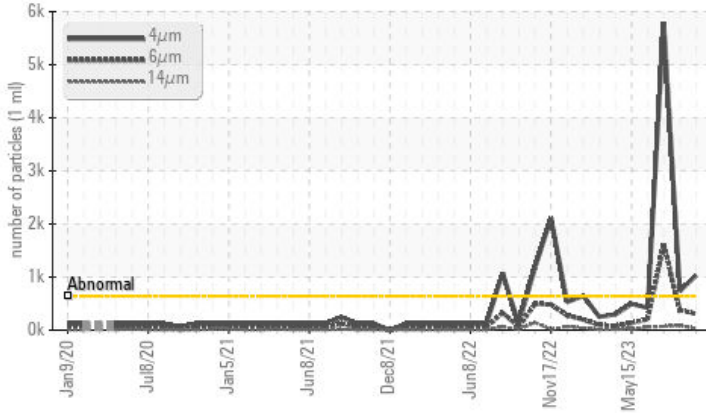

RECOMMENDATION

We recommend you service the filters on this component. Resample at the next service interval to monitor. Please note that this is a corrected copy for data entry updates.

PROBLEMATIC TEST RESULTS

| Sample Status | | | ATTENTION | ABNORMAL | SEVERE |
|-----------------|--------------|-----------|------------|------------|------------|
| Particles >4µm | ASTM D7647 | >640 | ▲ 1031 | ▲ 735 | ● 5797 |
| Particles >6µm | ASTM D7647 | >160 | ▲ 307 | ▲ 379 | ● 1619 |
| Particles >14µm | ASTM D7647 | >20 | ▲ 29 | ▲ 85 | ▲ 71 |
| Particles >21µm | ASTM D7647 | >4 | ▲ 9 | ▲ 35 | ▲ 21 |
| Oil Cleanliness | ISO 4406 (c) | >16/14/11 | ▲ 17/15/12 | ▲ 17/16/14 | ● 20/18/13 |

Customer Id: ALGSSM
 Sample No.: WC0837404
 Lab Number: 02586217
 Test Package: IND 2



To manage this report scan the QR code

To discuss the diagnosis or test data:
 Kevin Marson +1 (289)291-4644 x4644
Kevin.Marson@wearcheck.com

To change component or sample information:
 Gloria Gonzalez +1 (289)291-4643 x4643
gloria.gonzalez@wearcheck.com

RECOMMENDED ACTIONS

| Action | Status | Date | Done By | Description |
|---------------|--------|------|---------|---|
| Change Filter | --- | --- | ? | We recommend you service the filters on this component. |

HISTORICAL DIAGNOSIS

18 Aug 2023 Diag: Bill Quesnel

ISO



We advise that you perform a filter service, and use off-line filtration to improve the cleanliness of the system fluid. We recommend an early resample to monitor this condition. All component wear rates are normal. There is a moderate amount of particulates (2 to 100 microns in size) present in the oil. The system cleanliness is above the acceptable limit for the target ISO 4406 cleanliness code. The AN level is acceptable for this fluid. The pH level of this fluid is within the acceptable limits. The reserve alkalinity of this fluid is acceptable. The water concentration level is acceptable for this fluid. The oil is still serviceable provided that the contaminant(s) can be reduced to acceptable levels.

view report



ISO



08 Aug 2023 Diag: Kevin Marson

We advise that you check all areas where contaminants can enter the system. We advise that you perform a filter service, and use off-line filtration to improve the cleanliness of the system fluid. The air breather requires service. If unrated, we recommend that you replace with a suitable micron rated and/or desiccant air breather. If rated, we recommend that you service/replace the breather. Resample in 30-45 days to monitor this situation. All component wear rates are normal. There is a high amount of particulates (2 to 100 microns in size) present in the oil. The system cleanliness code is much higher than the acceptable limit for the target ISO 4406 cleanliness code. The AN level is acceptable for this fluid. The pH level of this fluid is within the acceptable limits. The reserve alkalinity of this fluid is acceptable. The water concentration level is acceptable for this fluid. The oil is still serviceable provided that the contaminant(s) can be reduced to acceptable levels.

view report



DEGRADATION



21 Jun 2023 Diag: Kevin Marson

Due to the low reserve alkalinity it is advised that you contact HOUGHTON to assist in restoring the proper amine concentration. We advise that you perform a filter service, and use off-line filtration to improve the cleanliness of the system fluid. We recommend an early resample to monitor this condition. All component wear rates are normal. There is a moderate amount of particulates (2 to 100 microns in size) present in the oil. The system cleanliness is above the acceptable limit for the target ISO 4406 cleanliness code. The reserve alkalinity of this fluid is lower than acceptable. The AN level is acceptable for this fluid. The pH level of this fluid is within the acceptable limits. The water concentration level is acceptable for this fluid. The oil is still serviceable provided that the contaminant(s) can be reduced to acceptable levels.


view report





OIL ANALYSIS REPORT

Sample Rating Trend

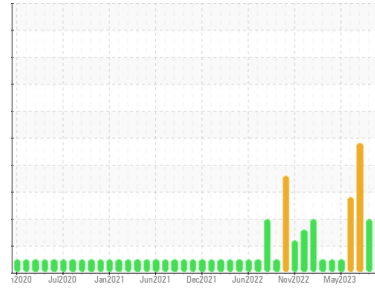

ISO



Area
Direct Strip Mill/Finishing
 Machine Id
PH3 HYDRAULIC SYSTEM (DSC004) (S/N 1000014662)
 Component
Hydraulic System
 Fluid
HOUGHTON HOUGHTO-SAFE 620 (15000 LTR)

DIAGNOSIS

Recommendation

We recommend you service the filters on this component. Resample at the next service interval to monitor. Please note that this is a corrected copy for data entry updates.

Wear

All component wear rates are normal.

Contamination

There is a light amount of silt (particulates < 14 microns in size) present in the oil.

Fluid Condition

The AN level is acceptable for this fluid. The pH level of this fluid is within the acceptable limits. The reserve alkalinity of this fluid is acceptable. The water concentration level is acceptable for this fluid. The condition of the oil is suitable for further service.

SAMPLE INFORMATION

| | method | limit/base | current | history1 | history2 |
|---------------|-------------|-------------|--------------------|-------------|-------------|
| Sample Number | Client Info | | WC0837404 | WC0780885 | WC0780830 |
| Sample Date | Client Info | | 26 Sep 2023 | 18 Aug 2023 | 08 Aug 2023 |
| Machine Age | hrs | Client Info | 0 | 0 | 0 |
| Oil Age | hrs | Client Info | 0 | 0 | 0 |
| Oil Changed | Client Info | | N/A | N/A | N/A |
| Sample Status | | | ATTENTION | ABNORMAL | SEVERE |

WEAR METALS

| | method | limit/base | current | history1 | history2 | |
|-----------|--------|---------------|---------|--------------|----------|----|
| Iron | ppm | ASTM D5185(m) | >40 | 0 | 0 | 0 |
| Chromium | ppm | ASTM D5185(m) | >4 | 0 | 0 | 0 |
| Nickel | ppm | ASTM D5185(m) | >20 | 0 | 0 | 0 |
| Titanium | ppm | ASTM D5185(m) | | 0 | 0 | 0 |
| Silver | ppm | ASTM D5185(m) | | <1 | <1 | 2 |
| Aluminum | ppm | ASTM D5185(m) | >4 | 0 | 0 | 0 |
| Lead | ppm | ASTM D5185(m) | >10 | 0 | 0 | 0 |
| Copper | ppm | ASTM D5185(m) | >60 | 0 | 0 | <1 |
| Tin | ppm | ASTM D5185(m) | >4 | 0 | 0 | 0 |
| Antimony | ppm | ASTM D5185(m) | | 0 | 0 | <1 |
| Vanadium | ppm | ASTM D5185(m) | | 0 | 0 | 0 |
| Beryllium | ppm | ASTM D5185(m) | | 0 | 0 | 0 |
| Cadmium | ppm | ASTM D5185(m) | | 0 | 0 | 0 |

ADDITIVES

| | method | limit/base | current | history1 | history2 | |
|------------|--------|---------------|---------|--------------|----------|----|
| Boron | ppm | ASTM D5185(m) | | <1 | 1 | 3 |
| Barium | ppm | ASTM D5185(m) | | <1 | 0 | 1 |
| Molybdenum | ppm | ASTM D5185(m) | | 0 | 0 | 0 |
| Manganese | ppm | ASTM D5185(m) | | 0 | 0 | 0 |
| Magnesium | ppm | ASTM D5185(m) | | <1 | <1 | 2 |
| Calcium | ppm | ASTM D5185(m) | | 0 | <1 | 2 |
| Phosphorus | ppm | ASTM D5185(m) | | 0 | <1 | 2 |
| Zinc | ppm | ASTM D5185(m) | | 0 | 0 | 0 |
| Sulfur | ppm | ASTM D5185(m) | | 38 | 53 | 56 |
| Lithium | ppm | ASTM D5185(m) | | 0 | <1 | <1 |

CONTAMINANTS






| | method | limit/base | current | history1 | history2 | |
|-----------|--------|---------------|---------|---------------|----------|--------|
| Silicon | ppm | ASTM D5185(m) | >20 | <1 | 0 | <1 |
| Sodium | ppm | ASTM D5185(m) | | 17 | <1 | 14 |
| Potassium | ppm | ASTM D5185(m) | >20 | 6 | <1 | 19 |
| Water | % | ASTM D6304* | >43.5 | 39.9 | 39.51 | 33.0 |
| ppm Water | ppm | ASTM D6304* | >435000 | 399000 | 395178.3 | 330000 |

FLUID CLEANLINESS

| | method | limit/base | current | history1 | history2 |
|-----------------|--------------|------------|-------------------|------------|------------|
| Particles >4µm | ASTM D7647 | >640 | ▲ 1031 | ▲ 735 | ● 5797 |
| Particles >6µm | ASTM D7647 | >160 | ▲ 307 | ▲ 379 | ● 1619 |
| Particles >14µm | ASTM D7647 | >20 | ▲ 29 | ▲ 85 | ▲ 71 |
| Particles >21µm | ASTM D7647 | >4 | ▲ 9 | ▲ 35 | ▲ 21 |
| Particles >38µm | ASTM D7647 | >3 | 0 | 2 | ▲ 6 |
| Particles >71µm | ASTM D7647 | >3 | 0 | 0 | 0 |
| Oil Cleanliness | ISO 4406 (c) | >16/14/11 | ▲ 17/15/12 | ▲ 17/16/14 | ● 20/18/13 |



OIL ANALYSIS REPORT

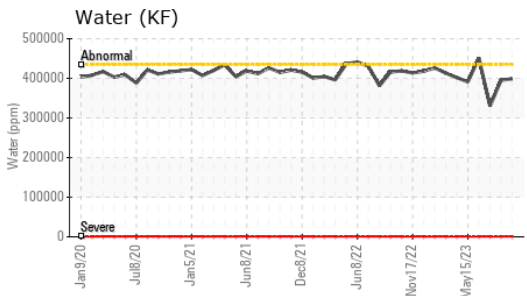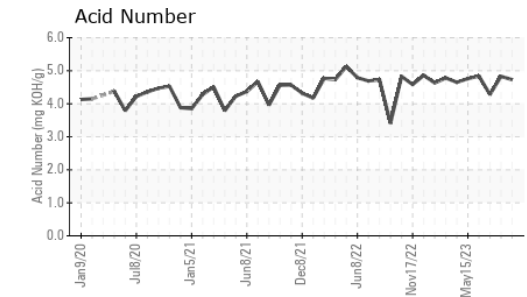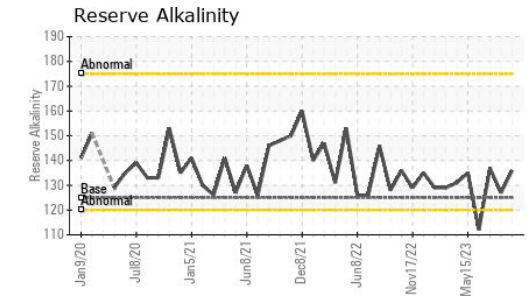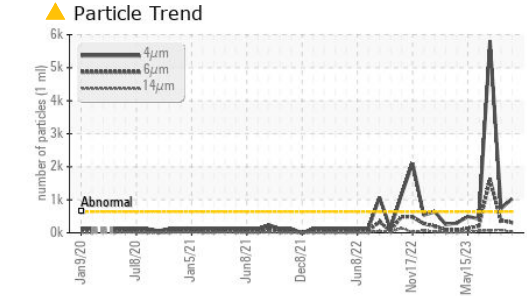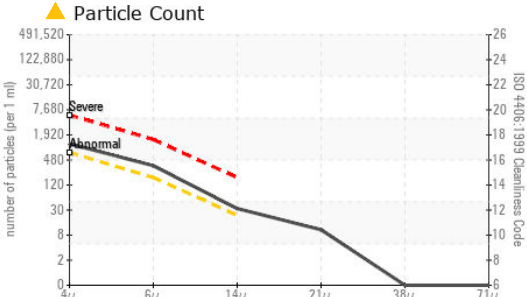


| FLUID DEGRADATION | | method | limit/base | current | history1 | history2 |
|-------------------------|----------|-------------|------------|-------------|----------|----------|
| Acid Number (AN) | mg KOH/g | ASTM D974* | | 4.73 | 4.83 | 4.28 |
| Alkiline Reserve (Oils) | ml KOH/g | ASTM D1121* | 125 | 136 | 127 | 137 |

| VISUAL | | method | limit/base | current | history1 | history2 |
|------------------|--------|---------|------------|----------------|----------|----------|
| White Metal | scalar | Visual* | NONE | NONE | NONE | NONE |
| Yellow Metal | scalar | Visual* | NONE | NONE | NONE | NONE |
| Precipitate | scalar | Visual* | NONE | NONE | NONE | NONE |
| Silt | scalar | Visual* | NONE | NONE | NONE | NONE |
| Debris | scalar | Visual* | NONE | NONE | NONE | NONE |
| Sand/Dirt | scalar | Visual* | NONE | NONE | NONE | NONE |
| Appearance | scalar | Visual* | NORML | FRGLY | FRGLY | FRGLY |
| Odor | scalar | Visual* | NORML | NORML | NORML | NORML |
| Emulsified Water | scalar | Visual* | >43.5 | >10% | >10% | >10% |
| Free Water | scalar | Visual* | | NEG | NEG | NEG |

| FLUID PROPERTIES | | method | limit/base | current | history1 | history2 |
|------------------|------------|---------------|------------|-------------|----------|----------|
| pH | Scale 0-14 | ASTM D1287* | | 9.39 | 9.43 | 9.62 |
| Visc @ 40°C | cSt | ASTM D7279(m) | | 41.2 | 42.1 | 41.5 |

| SAMPLE IMAGES | | method | limit/base | current | history1 | history2 |
|---------------|--|--------|------------|---------|----------|----------|
| Color | | | | | | |
| Bottom | | | | | | |

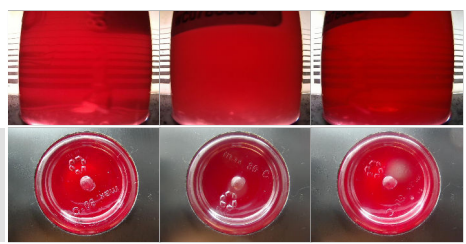

Laboratory : WearCheck - C8-1175 Appleby Line, Burlington, ON L7L 5H9 **ALGOMA STEEL INC. - STORES DEPT.**
Sample No. : WC0837404 **Received** : 02 Oct 2023
Lab Number : **02586217** **Diagnosed** : 13 Oct 2023
Unique Number : 5655283 **Diagnostician** : Kevin Marson
Test Package : IND 2 (Additional Tests: KF, pH, ReserveAlk, TAN Man)

301 WALLACE TERRACE
 SAULT STE MARIE, ON
 CA P6C 1K8
 Contact: Algoma Reliability
 algomareliability@algoma.com
 T: (705)206-1059
 F: (705)945-3585

To discuss this sample report, contact Customer Service at 1-800-268-2131.
 Test denoted (*) outside scope of accreditation, (m) method modified, (e) tested at external lab.
 Validity of results and interpretation are based on the sample and information as supplied.