

PROBLEM SUMMARY

Sample Rating Trend




PRESS 2 MAIN

Component

Hydraulic System

AW HYDRAULIC OIL ISO 46 (11000 LTR)

COMPONENT CONDITION SUMMARY

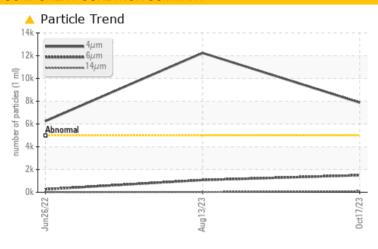

RECOMMENDATION

We recommend you service the filters on this component. Resample at the next service interval to monitor. Please specify the brand, type, and viscosity of the oil on your next sample. Please contact your representative for information regarding the proper sampling kits for your service. NOTE: We recommend using Advanced Oil Monitoring (AOM) kits for this system. The AOM test package includes advanced level testing to determine the suitability of turbine and large industrial compressor oils for continued use.

PROBLEMATIC T	EST RESULTS				
Sample Status			ATTENTION	ABNORMAL	ATTENTION
Particles >4µm	ASTM D7647	>5000	<u> </u>	<u>12242</u>	<u>▲</u> 6248
Particles >6µm	ASTM D7647	>1300	<u> </u>	1074	260
Oil Cleanliness	ISO 4406 (c)	>19/17/14	<u>^</u> 20/18/14	<u>\</u> 21/17/12	2 0/15/10

Customer Id: INDMIS Sample No.: WC Lab Number: 02590054 Test Package: IND 2



To manage this report scan the QR code

To discuss the diagnosis or test data: Wes Davis +1 905-569-8600 x223 wesd@wearcheck.ca

To change component or sample information: Gloria Gonzalez +1 (289)291-4643 x4643 gloria.gonzalez@wearcheck.com

RECOMMENDED ACTIONS

Action	Status	Date	Done By	Description
Change Filter			?	We recommend you service the filters on this component.
Contact Required			?	Please contact your representative for information regarding the proper sampling kits for your service.
Alert			?	NOTE: We recommend using Advanced Oil Monitoring (AOM) kits for this system. The AOM test package includes advanced level testing to determine the suitability of turbine and large industrial compressor oils for continued use.
Information Required			?	Please specify the brand, type, and viscosity of the oil on your next sample.

HISTORICAL DIAGNOSIS



13 Aug 2023 Diag: Wes Davis

We recommend you service the filters on this component. We recommend an early resample to monitor this condition. Please specify the brand, type, and viscosity of the oil on your next sample. Please contact your representative for information regarding the proper sampling kits for your service. NOTE: We recommend using Advanced Oil Monitoring (AOM) kits for this system. The AOM test package includes advanced level testing to determine the suitability of turbine and large industrial compressor oils for continued use. All component wear rates are normal. There is a moderate amount of silt (particulates < 14 microns in size) present in the oil. The AN level is acceptable for this fluid. The condition of the oil is acceptable for the time in service (unconfirmed). The oil is still serviceable provided that the contaminant(s) can be reduced to acceptable levels.





26 Jun 2022 Diag: Kevin Marson

Little or no information is provided as to the component and lubricant being tested. Recommendations are therefore generic in nature and may not apply to the current application. Please forward information as to equipment type, reservoir capacity, lubricant type and any pertinent information to allow for a more accurate assessment. We recommend you service the filters on this component. Resample at the next service interval to monitor. NOTE: Please provide information regarding reservoir capacity, filter type and micron rating with next sample. Please specify the brand, type, and viscosity of the oil on your next sample. All component wear rates are normal. There is a light amount of silt (particulates < 14 microns in size) present in the oil. The AN level is acceptable for this fluid. The condition of the oil is suitable for further service.



Report Id: INDMIS [WCAMIS] 02590054 (Generated: 10/19/2023 08:54:11) Rev: 1



OIL ANALYSIS REPORT

Sample Rating Trend

ISO



PRESS 2 MAIN

Component

Hydraulic System

AW HYDRAULIC OIL ISO 46 (11000 LTR)

DIAGNOSIS

Recommendation

We recommend you service the filters on this component. Resample at the next service interval to monitor. Please specify the brand, type, and viscosity of the oil on your next sample. Please contact your representative for information regarding the proper sampling kits for your service. NOTE: We recommend using Advanced Oil Monitoring (AOM) kits for this system. The AOM test package includes advanced level testing to determine the suitability of turbine and large industrial compressor oils for continued use.

Wear

All component wear rates are normal.

Contamination

There is a light amount of silt (particulates < 14 microns in size) present in the oil.

Fluid Condition

The AN level is acceptable for this fluid. The condition of the oil is acceptable for the time in service (unconfirmed).


		Jui	n2022	Aug2023	Oct2023	
SAMPLE INFORM	MATION	method	limit/base	current	history1	history2
Sample Number		Client Info		wc	WC	WC
Sample Date		Client Info		17 Oct 2023	13 Aug 2023	26 Jun 2022
Machine Age	hrs	Client Info		0	0	0
Oil Age	hrs	Client Info		0	0	0
Oil Changed		Client Info		N/A	N/A	N/A
Sample Status				ATTENTION	ABNORMAL	ATTENTION
WEAR METALS		method	limit/base	current	history1	history2
Iron	ppm	ASTM D5185(m)	>20	3	3	2
Chromium	ppm	ASTM D5185(m)	>20	0	0	0
Nickel	ppm	ASTM D5185(m)	>20	<1	0	0
Titanium	ppm	ASTM D5185(m)		0	0	0
Silver	ppm	ASTM D5185(m)		<1	0	0
Aluminum	ppm	ASTM D5185(m)	>20	0	<1	0
Lead	ppm	ASTM D5185(m)	>20	<1	<1	1
Copper	ppm	ASTM D5185(m)	>20	14	14	15
Tin	ppm	ASTM D5185(m)	>20	0	0	0
Antimony	ppm	ASTM D5185(m)		0	0	0
Vanadium	ppm	ASTM D5185(m)		0	0	0
Beryllium	ppm	ASTM D5185(m)		0	0	0
Cadmium	ppm	ASTM D5185(m)		0	0	0
ADDITIVES		method	limit/base	current	history1	history2
Boron	ppm	ASTM D5185(m)	5	<1	<1	<1
Barium	ppm	ASTM D5185(m)		<1	0	0
Molybdenum	ppm	ASTM D5185(m)	5	0	0	0
Manganese	ppm	ASTM D5185(m)		0	0	0
Magnesium	ppm	ASTM D5185(m)	25	<1	1	1
Calcium	ppm	ASTM D5185(m)	200	60	59	59
Phosphorus	ppm	ASTM D5185(m)	300	341	368	324
Zinc	ppm	ASTM D5185(m)	370	430	437	405
Sulfur	ppm	ASTM D5185(m)	2500	753	769	762
Lithium	ppm	ASTM D5185(m)	2000	<1	<1	<1
CONTAMINANTS		method	limit/base	current	history1	history2
Silicon		ASTM D5185(m)	>15	0	<1	0
Sodium	ppm	ASTM D5185(m)	710	<1	<1	<1
Potassium	ppm	ASTM D5185(m)	>20	0	<1	0
FLUID CLEANLIN		method	limit/base	current	history1	history2
Particles >4µm		ASTM D7647	>5000	▲ 7877	<u> 12242</u>	▲ 6248
Particles >6µm		ASTM D7647	>1300	1498	1074	260
Particles >14µm		ASTM D7647	>160	102	23	10
Particles >21µm		ASTM D7647		26	6	2
Particles >38µm		ASTM D7647	>10	2	0	1
Particles >71µm		ASTM D7647		0	0	0
Oil Cleanliness		ISO 4406 (c)	>19/17/14	<u>^</u> 20/18/14	△ 21/17/12	<u>^</u> 20/15/10
FLUID DEGRADA	TION	method	limit/base			
I LOID DEGRADA	TION	method	mmi/pase	current	history1	history2

0.26

0.39



OIL ANALYSIS REPORT

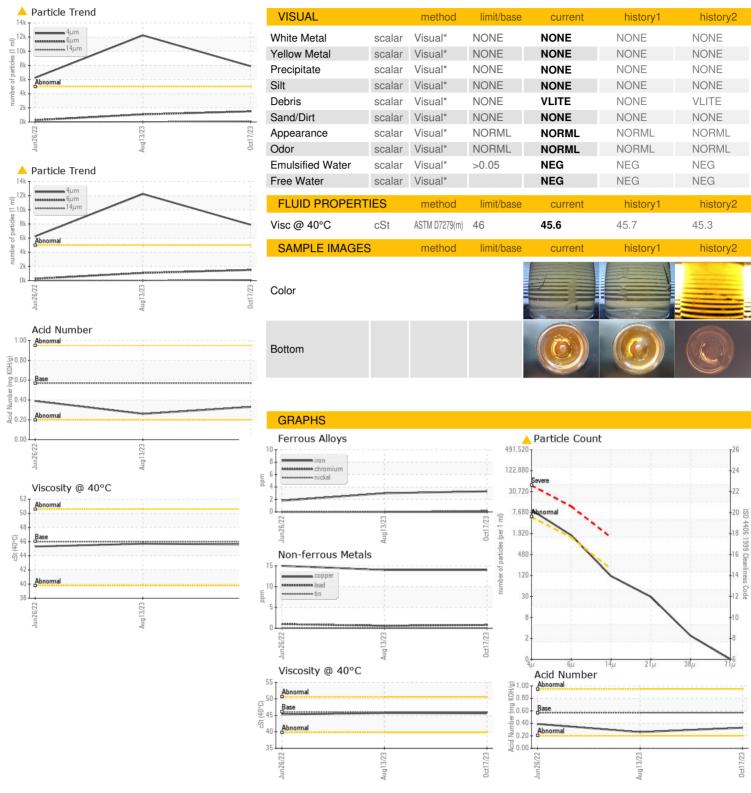



CALA ISO 17025:2017 Accredited Laboratory

Laboratory Sample No. Lab Number

Unique Number

Test Package

: WC

02590054 : 5659120 : IND 2

: WearCheck - C8-1175 Appleby Line, Burlington, ON L7L 5H9 : 18 Oct 2023 Received Diagnosed : 19 Oct 2023 Diagnostician

: Wes Davis

To discuss this sample report, contact Customer Service at 1-800-268-2131. Test denoted (*) outside scope of accreditation, (m) method modified, (e) tested at external lab. Validity of results and interpretation are based on the sample and information as supplied.

Hydro Extrusion North 5675 Kennedy Road

Mississauga, ON CA L4Z 2H9 Contact: Harsh Murria Harsh.murria@hydro.com T: (819)462-0479

F: (866)462-6478