




# OIL ANALYSIS REPORT

Sample Rating Trend

**NORMAL**

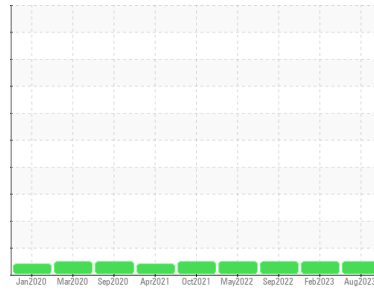

Area  
**DRYERS**  
 Machine Id  
**C-645**  
 Component  
**Gearbox**  
 Fluid  
**MOBIL SHC 630 (4 LTR)**

## DIAGNOSIS

### Recommendation

Resample at the next service interval to monitor.

### Wear

All component wear rates are normal.

### Contamination

There is no indication of any contamination in the oil. The amount and size of particulates present in the system are acceptable.

### Fluid Condition

The AN level is acceptable for this fluid. The condition of the oil is suitable for further service.

## SAMPLE INFORMATION

	method	limit/base	current	history1	history2
Sample Number	Client Info		<b>WC0849088</b>	WC0788662	WC0739607
Sample Date	Client Info		<b>17 Aug 2023</b>	09 Feb 2023	14 Sep 2022
Machine Age	yrs	Client Info	<b>5</b>	5	5
Oil Age	yrs	Client Info	<b>3</b>	3	3
Oil Changed	Client Info		<b>N/A</b>	Not Changd	Not Changd
Sample Status			<b>NORMAL</b>	NORMAL	NORMAL

## WEAR METALS

	method	limit/base	current	history1	history2
Iron	ppm	ASTM D5185m >200	<b>&lt;1</b>	1	1
Chromium	ppm	ASTM D5185m >15	<b>0</b>	0	0
Nickel	ppm	ASTM D5185m >15	<b>&lt;1</b>	0	0
Titanium	ppm	ASTM D5185m	<b>0</b>	0	0
Silver	ppm	ASTM D5185m	<b>0</b>	0	<1
Aluminum	ppm	ASTM D5185m >25	<b>0</b>	0	<1
Lead	ppm	ASTM D5185m >100	<b>&lt;1</b>	0	0
Copper	ppm	ASTM D5185m >200	<b>0</b>	0	0
Tin	ppm	ASTM D5185m >25	<b>0</b>	0	<1
Vanadium	ppm	ASTM D5185m	<b>0</b>	0	0
Cadmium	ppm	ASTM D5185m	<b>0</b>	0	0

## ADDITIVES

	method	limit/base	current	history1	history2
Boron	ppm	ASTM D5185m	<b>0</b>	0	0
Barium	ppm	ASTM D5185m	<b>0</b>	0	0
Molybdenum	ppm	ASTM D5185m	<b>0</b>	0	0
Manganese	ppm	ASTM D5185m	<b>0</b>	0	0
Magnesium	ppm	ASTM D5185m	<b>&lt;1</b>	<1	0
Calcium	ppm	ASTM D5185m	<b>0</b>	3	1
Phosphorus	ppm	ASTM D5185m	<b>437</b>	392	438
Zinc	ppm	ASTM D5185m	<b>0</b>	<1	1
Sulfur	ppm	ASTM D5185m	<b>15</b>	83	56

## CONTAMINANTS

	method	limit/base	current	history1	history2
Silicon	ppm	ASTM D5185m >50	<b>32</b>	9	11
Sodium	ppm	ASTM D5185m	<b>0</b>	0	0
Potassium	ppm	ASTM D5185m >20	<b>&lt;1</b>	0	0

## FLUID CLEANLINESS

	method	limit/base	current	history1	history2
Particles >4µm	ASTM D7647	>20000	<b>5341</b>	5103	---
Particles >6µm	ASTM D7647	>5000	<b>1398</b>	1363	---
Particles >14µm	ASTM D7647	>640	<b>82</b>	107	---
Particles >21µm	ASTM D7647	>160	<b>16</b>	28	---
Particles >38µm	ASTM D7647	>40	<b>0</b>	8	---
Particles >71µm	ASTM D7647	>10	<b>0</b>	1	---
Oil Cleanliness	ISO 4406 (c)	>21/19/16	<b>20/18/14</b>	20/18/14	---


## FLUID DEGRADATION

	method	limit/base	current	history1	history2
Acid Number (AN)	mg KOH/g	ASTM D8045	<b>0.44</b>	0.29	0.32




# OIL ANALYSIS REPORT


**Particle Trend**

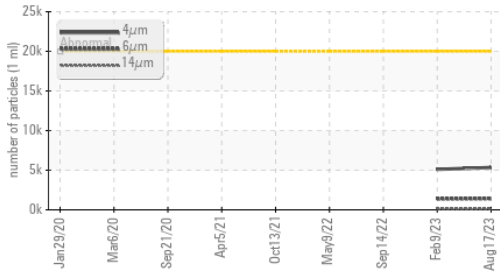


**Acid Number**

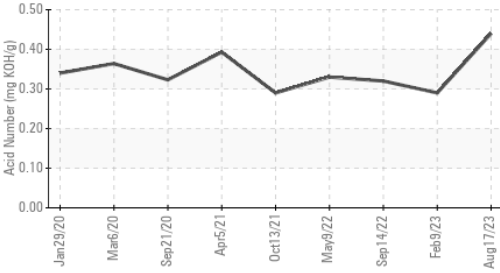

**Viscosity @ 40°C**

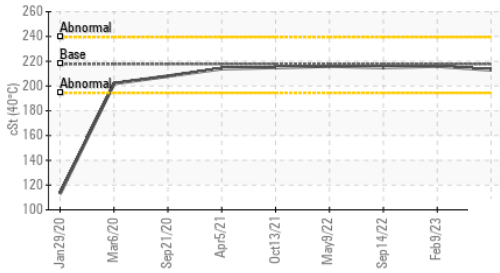


**Particle Trend**

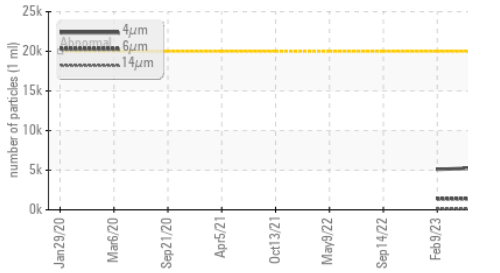

VISUAL	method	limit/base	current	history1	history2
White Metal	scalar	*Visual	NONE	NONE	NONE
Yellow Metal	scalar	*Visual	NONE	NONE	NONE
Precipitate	scalar	*Visual	NONE	NONE	NONE
Silt	scalar	*Visual	NONE	NONE	NONE
Debris	scalar	*Visual	NONE	NONE	NONE
Sand/Dirt	scalar	*Visual	NONE	NONE	NONE
Appearance	scalar	*Visual	NORML	NORML	NORML
Odor	scalar	*Visual	NORML	NORML	NORML
Emulsified Water	scalar	*Visual	>0.2	NEG	NEG
Free Water	scalar	*Visual		NEG	NEG


FLUID PROPERTIES	method	limit/base	current	history1	history2	
Visc @ 40°C	cSt	ASTM D445	217.7	<b>213</b>	216	215

SAMPLE IMAGES	method	limit/base	current	history1	history2
---------------	--------	------------	---------	----------	----------

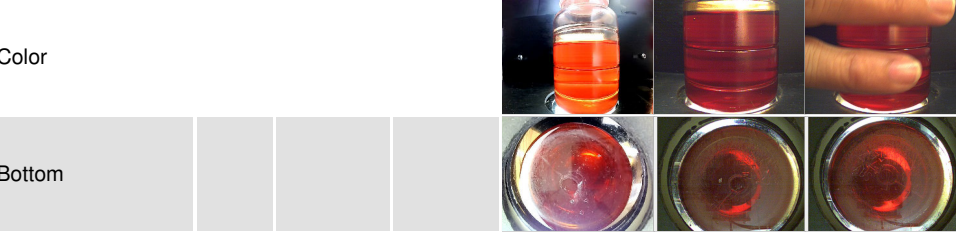


## GRAPHS


**Ferrous Alloys**

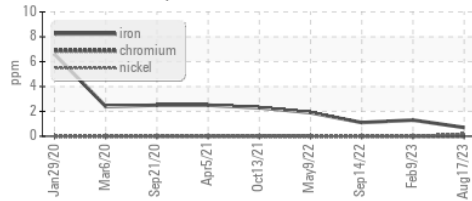


**Non-ferrous Metals**

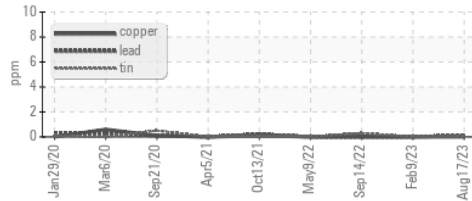


**Viscosity @ 40°C**

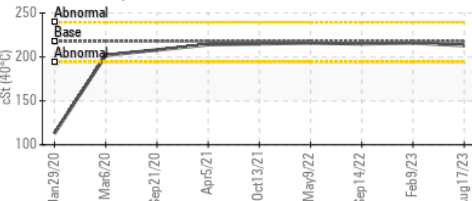

**Particle Count**

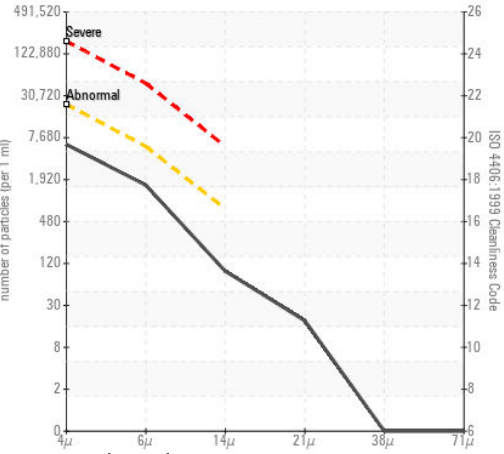

**Acid Number**

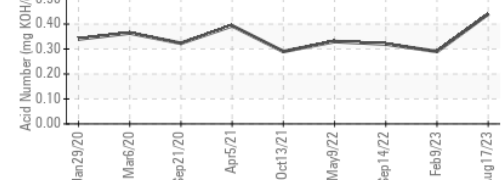

**Laboratory** : WearCheck USA - 501 Madison Ave., Cary, NC 27513  
**Sample No.** : WC0849088 **Received** : 21 Aug 2023  
**Lab Number** : 05929823 **Diagnosed** : 24 Aug 2023  
**Unique Number** : 10615094 **Diagnostician** : Doug Bogart  
**Test Package** : IND 2 ( Additional Tests: PrtCount )

**POET BIOREFINING - Groton**  
 40425 133RD STREET  
 GROTON, SD  
 US 57445-6400  
 Contact: GAVIN KRUEGER  
 Gavin.Krueger@POET.COM  
 T: 6(05) 846-6863  
 F: (605)397-2754

Certificate L2367  
 To discuss this sample report, contact Customer Service at 1-800-237-1369.  
 \* - Denotes test methods that are outside of the ISO 17025 scope of accreditation.  
 Statements of conformity to specifications are based on the simple acceptance decision rule (JCGM 106:2012)