



PROBLEM SUMMARY

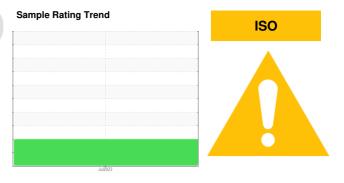

KAESER 5465785 (S/N 1407)

Compressor Fluid KAESER SIGMA (OEM) M-460 (--- QTS)

COMPONENT CONDITION SUMMARY

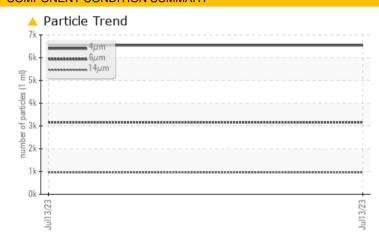

RECOMMENDATION

No corrective action is recommended at this time. The filter change at the time of sampling has been noted. Resample at the next service interval to monitor.

PROBLEMATIC TEST RESULTS

| Sample Status | | ABNORMAL | | | | | | |
|-----------------|----------------|-------------------|--|--|--|--|--|--|
| Particles >6µm | ASTM D7647 >1 | 300 🔺 3161 | | | | | | |
| Particles >14µm | ASTM D7647 >8 | D 🔺 952 | | | | | | |
| Particles >21µm | ASTM D7647 >2 | 0 🔺 493 | | | | | | |
| Particles >38µm | ASTM D7647 >4 | <u> </u> | | | | | | |
| Oil Cleanliness | ISO 4406 (c) > | /17/13 🔺 20/19/17 | | | | | | |

Customer Id: SUDWIG Sample No.: KC05935409 Lab Number: 05935409 Test Package: IND 2



To manage this report scan the QR code

To discuss the diagnosis or test data: Don Baldridge +1 <u>don.b505@comcast.net</u>

To change component or sample information: Customer Service +1 1-800-237-1369 <u>customerservice@wearcheck.com</u> There are no recommended actions for this sample.

HISTORICAL DIAGNOSIS



OIL ANALYSIS REPORT



ISO

KAESER 5465785 (S/N 1407)

Compressor Fluid KAESER SIGMA (OEM) M-460 (--- QTS)

DIAGNOSIS

Recommendation

No corrective action is recommended at this time. The filter change at the time of sampling has been noted. Resample at the next service interval to monitor.

Wear

All component wear rates are normal.

Contamination

There is a high amount of particulates present in the oil.

Fluid Condition

The AN level is acceptable for this fluid. The condition of the oil is acceptable for the time in service.

| SAMPLE INFORM | ATION | method | limit/base | current | history1 | history2 |
|------------------|----------|--------------|------------|-------------------|----------|----------|
| Sample Number | | Client Info | | KC05935409 | | |
| Sample Date | | Client Info | | 13 Jul 2023 | | |
| Machine Age | hrs | Client Info | | 8194 | | |
| Oil Age | hrs | Client Info | | 0 | | |
| Oil Changed | | Client Info | | N/A | | |
| Sample Status | | | | ABNORMAL | | |
| WEAR METALS | | method | limit/base | current | history1 | history2 |
| Iron | ppm | ASTM D5185m | >50 | 0 | | |
| Chromium | ppm | ASTM D5185m | >10 | 0 | | |
| Nickel | ppm | ASTM D5185m | >3 | 0 | | |
| Titanium | ppm | ASTM D5185m | >3 | 0 | | |
| Silver | ppm | ASTM D5185m | >2 | 0 | | |
| Aluminum | ppm | ASTM D5185m | >10 | 0 | | |
| Lead | ppm | ASTM D5185m | >10 | 0 | | |
| Copper | ppm | ASTM D5185m | >50 | 33 | | |
| Tin | ppm | ASTM D5185m | >10 | 0 | | |
| Vanadium | ppm | ASTM D5185m | | <1 | | |
| Cadmium | ppm | ASTM D5185m | | 0 | | |
| ADDITIVES | | method | limit/base | current | history1 | history2 |
| Boron | ppm | ASTM D5185m | 0 | 0 | | |
| Barium | ppm | ASTM D5185m | 90 | 0 | | |
| Molybdenum | ppm | ASTM D5185m | 0 | 0 | | |
| Manganese | ppm | ASTM D5185m | 0 | 0 | | |
| Magnesium | ppm | ASTM D5185m | 100 | 0 | | |
| Calcium | ppm | ASTM D5185m | 0 | 0 | | |
| Phosphorus | ppm | ASTM D5185m | 0 | 0 | | |
| Zinc | ppm | ASTM D5185m | | 0 | | |
| - | | | | Ū | | |
| CONTAMINANTS | | method | limit/base | current | history1 | history2 |
| Silicon | ppm | ASTM D5185m | >25 | <1 | | |
| Sodium | ppm | ASTM D5185m | | 1 | | |
| Potassium | ppm | ASTM D5185m | >20 | 0 | | |
| Water | % | ASTM D6304 | | 0.011 | | |
| ppm Water | ppm | ASTM D6304 | >500 | 114.0 | | |
| FLUID CLEANLIN | IESS | method | limit/base | current | history1 | history2 |
| Particles >4µm | | ASTM D7647 | | 6546 | | |
| Particles >6µm | | ASTM D7647 | | A 3161 | | |
| Particles >14µm | | ASTM D7647 | >80 | A 952 | | |
| Particles >21µm | | ASTM D7647 | | 493 | | |
| Particles >38µm | | ASTM D7647 | >4 | 4 1 | | |
| Particles >71µm | | ASTM D7647 | | 2 | | |
| Oil Cleanliness | | ISO 4406 (c) | >/17/13 | A 20/19/17 | | |
| FLUID DEGRADA | TION | method | limit/base | current | history1 | history2 |
| Acid Number (AN) | mg KOH/g | ASTM D8045 | 1.0 | 0.30 | | |



OIL ANALYSIS REPORT

method


limit/base

current


history1


history2

VISUAL





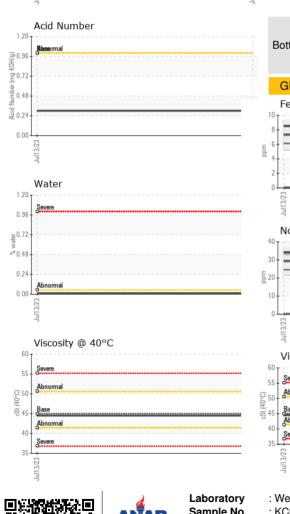


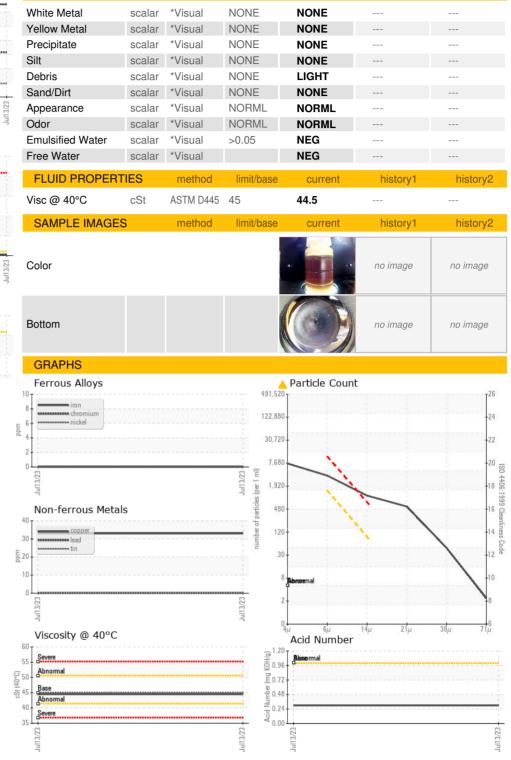

: 25 Aug 2023

: 28 Aug 2023

: Don Baldridge



* - Denotes test methods that are outside of the ISO 17025 scope of accreditation.

Statements of conformity to specifications are based on the simple acceptance decision rule (JCGM 106:2012)

Received

Diagnosed

Diagnostician

Contact/Location: Service Manager - SUDWIG

SUDDEN IMPACT COLLISION

664 W FRONTAGE DR

Contact: Service Manager

WIGGINS, MS

US 39577