

# **PROBLEM SUMMARY**

Sample Rating Trend




KAESER 7907156

Component

Compressor

KAESER SIGMA (OEM) M-460 (--- GAL)

# **COMPONENT CONDITION SUMMARY**

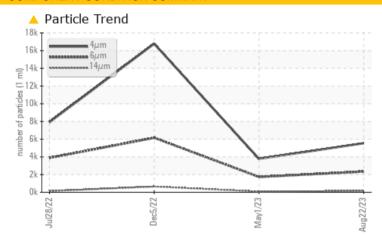

# RECOMMENDATION

No corrective action is recommended at this time. Oil and filter change at the time of sampling has been noted. Resample at the next service interval to monitor.

PROBLEMATIC TEST F	RESULTS				
Sample Status			ATTENTION	ATTENTION	ABNORMAL
Particles >6µm	ASTM D7647	>1300	<b>2345</b>	<u>▲</u> 1732	<u></u> 6160
Particles >14μm	ASTM D7647	>80	<b>155</b>	<u></u> 85	<b>△</b> 648
Particles >21µm	ASTM D7647	>20	<u> </u>	9	<u>^</u> 276
Oil Cleanliness	ISO 4406 (c)	>/17/13	<b>20/18/14</b>	19/18/14	▲ 21/20/17

Customer Id: AMACOL Sample No.: KCPA003599 Lab Number: 05938314 Test Package: IND 2



To manage this report scan the QR code

To discuss the diagnosis or test data: Doug Bogart +1 (800)237-1369 x4016 dougb@wearcheckusa.com

To change component or sample information: Customer Service +1 1-800-237-1369 customerservice@wearcheck.com

# **RECOMMENDED ACTIONS**

Action	Status	Date	Done By	Description
Change Fluid			?	Oil and filter change at the time of sampling has been noted.
Change Filter			?	Oil and filter change at the time of sampling has been noted.

# HISTORICAL DIAGNOSIS

# 01 May 2023 Diag: Angela Borella





Oil and filter change at the time of sampling has been noted. Resample at the next service interval to monitor. All component wear rates are normal. There is a moderate amount of silt (particulates < 14 microns in size) present in the oil. The BN result indicates that there is suitable alkalinity remaining in the oil. The condition of the oil is suitable for further service.



# 05 Dec 2022 Diag: Jonathan Hester

ISO



Oil and filter change at the time of sampling has been noted. Resample at the next service interval to monitor. All component wear rates are normal. There is a high amount of particulates present in the oil. The AN level is acceptable for this fluid. The condition of the oil is suitable for further service.

# view report

# 28 Jul 2022 Diag: Angela Borella

ISO




Oil and filter change at the time of sampling has been noted. Resample at the next service interval to monitor. All component wear rates are normal. There is a high amount of silt (particulates < 14 microns in size) present in the oil. The BN result indicates that there is suitable alkalinity remaining in the oil. The condition of the oil is suitable for further service.





# **OIL ANALYSIS REPORT**

Sample Rating Trend



ISO



# **KAESER 7907156**

Component

Compressor

KAESER SIGMA (OEM) M-460 (--- GAL)

# **DIAGNOSIS**

# Recommendation

No corrective action is recommended at this time. Oil and filter change at the time of sampling has been noted. Resample at the next service interval to monitor.

# Wear

All component wear rates are normal.

# Contamination

There is a moderate amount of particulates present in the oil.

# **Fluid Condition**

The BN result indicates that there is suitable alkalinity remaining in the oil. The condition of the oil is suitable for further service.

		Jul202	2 Dec2022	May2023 Au	g2023	
SAMPLE INFORM	MATION	method	limit/base	current	history1	history2
Sample Number		Client Info		KCPA003599	KCP53436	KCP49892
Sample Date		Client Info		22 Aug 2023	01 May 2023	05 Dec 2022
Machine Age	hrs	Client Info		0	4340	3040
Oil Age	hrs	Client Info		0	1301	1045
Oil Changed		Client Info		Changed	Changed	Changed
Sample Status				ATTENTION	ATTENTION	ABNORMAL
WEAR METALS		method	limit/base	current	history1	history2
Iron	ppm	ASTM D5185m	>50	<1	0	<1
Chromium	ppm	ASTM D5185m	>10	0	0	0
Nickel	ppm	ASTM D5185m	>3	0	0	0
Titanium	ppm	ASTM D5185m	>3	0	0	0
Silver	ppm	ASTM D5185m	>2	0	0	0
Aluminum	ppm	ASTM D5185m	>10	<1	0	0
Lead	ppm	ASTM D5185m	>10	0	0	0
Copper	ppm	ASTM D5185m	>50	<1	<1	<1
Tin	ppm	ASTM D5185m	>10	0	0	0
Vanadium	ppm	ASTM D5185m		0	0	0
Cadmium	ppm	ASTM D5185m		0	0	0
ADDITIVES		method	limit/base	current	history1	history2
Boron	ppm	ASTM D5185m	0	0	0	0
Barium	ppm	ASTM D5185m	90	12	76	34
Molybdenum	ppm	ASTM D5185m	0	0	0	0
Manganese	ppm	ASTM D5185m		0	0	0
Magnesium	ppm	ASTM D5185m	100	75	89	85
Calcium	ppm	ASTM D5185m	0	0	0	<1
Phosphorus	ppm	ASTM D5185m	0	<1	1	6
Zinc	ppm	ASTM D5185m	0	2	2	3
Sulfur	ppm	ASTM D5185m	23500	19834	21437	19410
CONTAMINANTS		method	limit/base	current	history1	history2
Silicon	ppm	ASTM D5185m	>25	<1	0	<1
Sodium	ppm	ASTM D5185m		6	7	10
Potassium	ppm	ASTM D5185m	>20	<1	1	2
Water	%	ASTM D6304	>0.05	0.025	0.012	0.008
ppm Water	ppm	ASTM D6304	>500	258.2	128.0	81.0
FLUID CLEANLIN	ESS	method	limit/base	current	history1	history2
Particles >4µm		ASTM D7647		5542	3781	16778
Particles >6µm		ASTM D7647	>1300	<b>2345</b>	<u>▲</u> 1732	<u></u> 6160
Particles >14µm		ASTM D7647	>80	<u> </u>	<u></u> 85	<b>△</b> 648
Particles >21µm		ASTM D7647	>20	<u> </u>	9	<u>^</u> 276
Particles >38µm		ASTM D7647	>4	1	1	<b>△</b> 35
Particles >71µm		ASTM D7647	>3	0	0	1
Oil Cleanliness		ISO 4406 (c)	>/17/13	<u>^</u> 20/18/14	▲ 19/18/14	<u>\$\text{\Delta}\$ 21/20/17</u>
FLUID DEGRADA	TION	method	limit/base	current	history1	history2



# **OIL ANALYSIS REPORT**







Sample No. Lab Number **Unique Number** 

: KCPA003599 : 05938314

Received Diagnosed : 10628926

: 31 Aug 2023 Diagnostician : Doug Bogart Test Package : IND 2 ( Additional Tests: KF, PrtCount )

Certificate L2367 To discuss this sample report, contact Customer Service at 1-800-237-1369.

\* - Denotes test methods that are outside of the ISO 17025 scope of accreditation. Statements of conformity to specifications are based on the simple acceptance decision rule (JCGM 106:2012)

**4222 INTERGRATIONS LOOP** COLORADO SPRINGS, CO

US 80916

Contact: Service Manager

T:

F: