

# **PROBLEM SUMMARY**

Sample Rating Trend


WEAR

TS03-08

Component **Hydraulic System** 

**DURA CLEAN (330 GAL)** 

# **COMPONENT CONDITION SUMMARY**

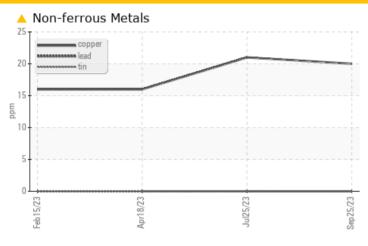

# RECOMMENDATION

No corrective action is recommended at this time. Resample at the next service interval to monitor.

PROBLEMATIC TEST RESULTS								
Sample Status				ABNORMAL	ABNORMAL	NORMAL		
Copper	ppm	ASTM D5185m	>20	<u>^</u> 20	<u>^</u> 21	16		
PrtFilter						no image		

Customer Id: PARCOR Sample No.: PH0001187 Lab Number: 05967765 Test Package: PLANT

To manage this report scan the QR code

To discuss the diagnosis or test data: Jonathan Hester +1 919-379-4092 x4092 jhester@wearcheckusa.com

To change component or sample information: Customer Service +1 1-800-237-1369 customerservice@wearcheck.com

# **RECOMMENDED ACTIONS**

There are no recommended actions for this sample.

# HISTORICAL DIAGNOSIS

# 25 Jul 2023 Diag: Jonathan Hester

WEAR



No corrective action is recommended at this time. Resample at the next service interval to monitor. The copper level is abnormal. All other component wear rates are normal. There is no indication of any contamination in the oil. The amount and size of particulates present in the system are acceptable. The AN level is acceptable for this fluid. The condition of the oil is suitable for further service.



### 18 Apr 2023 Diag: Don Baldridge

NORMAL



Resample at the next service interval to monitor. All component wear rates are normal. There is no indication of any contamination in the oil. The amount and size of particulates present in the system are acceptable. The AN level is acceptable for this fluid. The condition of the oil is suitable for further service.



## 15 Feb 2023 Diag: Doug Bogart

NORMAL



Resample at the next service interval to monitor. All component wear rates are normal. There is no indication of any contamination in the oil. The amount and size of particulates present in the system are acceptable. The AN level is acceptable for this fluid. The condition of the oil is suitable for further service.





# **OIL ANALYSIS REPORT**

**ADDITIVES** 

Sample Rating Trend





TS03-08

Component

**Hydraulic System** 

**DURA CLEAN (330 GAL)** 

# DIAGNOSIS

### Recommendation

No corrective action is recommended at this time. Resample at the next service interval to monitor.

The copper level is abnormal. All other component wear rates are normal.

### Contamination

There is no indication of any contamination in the oil. The amount and size of particulates present in the system are acceptable.

# **Fluid Condition**

The AN level is acceptable for this fluid. The condition of the oil is suitable for further service.

						<u> </u>
		Feb 2023	Apr2023	Jul2023 8	Sep 2023	
SAMPLE INFOR	MATION	method	limit/base	current	history1	history2
Sample Number		Client Info		PH0001187	PH0001185	PH05831115
Sample Date		Client Info		25 Sep 2023	25 Jul 2023	18 Apr 2023
Machine Age	hrs	Client Info		0	0	0
Oil Age	hrs	Client Info		0	0	0
Oil Changed		Client Info		N/A	N/A	N/A
Sample Status				ABNORMAL	ABNORMAL	NORMAL

WEAR METALS		method	limit/base	current	history1	history2
Iron	ppm	ASTM D5185m	>20	<1	<1	<1
Chromium	ppm	ASTM D5185m	>20	0	0	0
Nickel	ppm	ASTM D5185m	>20	0	0	0
Titanium	ppm	ASTM D5185m		0	0	0
Silver	ppm	ASTM D5185m		0	0	0
Aluminum	ppm	ASTM D5185m	>20	0	<1	0
Lead	ppm	ASTM D5185m	>20	0	0	0
Copper	ppm	ASTM D5185m	>20	<u>^</u> 20	<u>^</u> 21	16
Tin	ppm	ASTM D5185m	>20	0	0	0
Vanadium	ppm	ASTM D5185m		0	<1	0
Cadmium	ppm	ASTM D5185m		0	0	0

<b>Barium</b> ppm ASTM D5185m <b>0</b> 0 0	
Molybdenum ppm ASTM D5185m <b>0</b> 2 0	
Manganese ppm ASTM D5185m <b>0</b> <1 0	
<b>Magnesium</b> ppm ASTM D5185m <b>&lt;1</b> 0 <1	
Calcium ppm ASTM D5185m 26 21 22	
Phosphorus ppm ASTM D5185m 406 481 442	
<b>Zinc</b> ppm ASTM D5185m <b>588</b> 642 640	
Sulfur ppm ASTM D5185m 1265 1410 1155	

limit/base

current

method

CONTAMINANTS		method	limit/base	current	history1	history2
Silicon	ppm	ASTM D5185m	>15	<1	<1	0
Sodium	ppm	ASTM D5185m		0	2	0
Potassium	ppm	ASTM D5185m	>20	<1	0	<1
FLUID CLEA	NLINESS	method	limit/base	current	history1	history2
Partialas - 1um		ACTM D7647	- 10000	2105	10/11	906

Particles >4µm	ASTM D7647	>10000	2105	1241	896
Particles >6µm	ASTM D7647	>2500	353	258	173
Particles >14μm	ASTM D7647	>320	11	28	8
Particles >21µm	ASTM D7647	>80	1	7	2
Particles >38μm	ASTM D7647	>20	0	0	0
Particles >71µm	ASTM D7647	>4	0	0	0
Oil Cleanliness	ISO 4406 (c)	>20/18/15	18/16/11	17/15/12	17/15/10
FILLID DEODADATION	41.0	12 24 0		1111	1110

FLUID DEGRADA	ATION	method	iiiiii/base	current	riistory i	HIStory
Acid Number (AN)	mg KOH/g	ASTM D8045		0.50	0.59	0.55




history1

history2



# **OIL ANALYSIS REPORT**

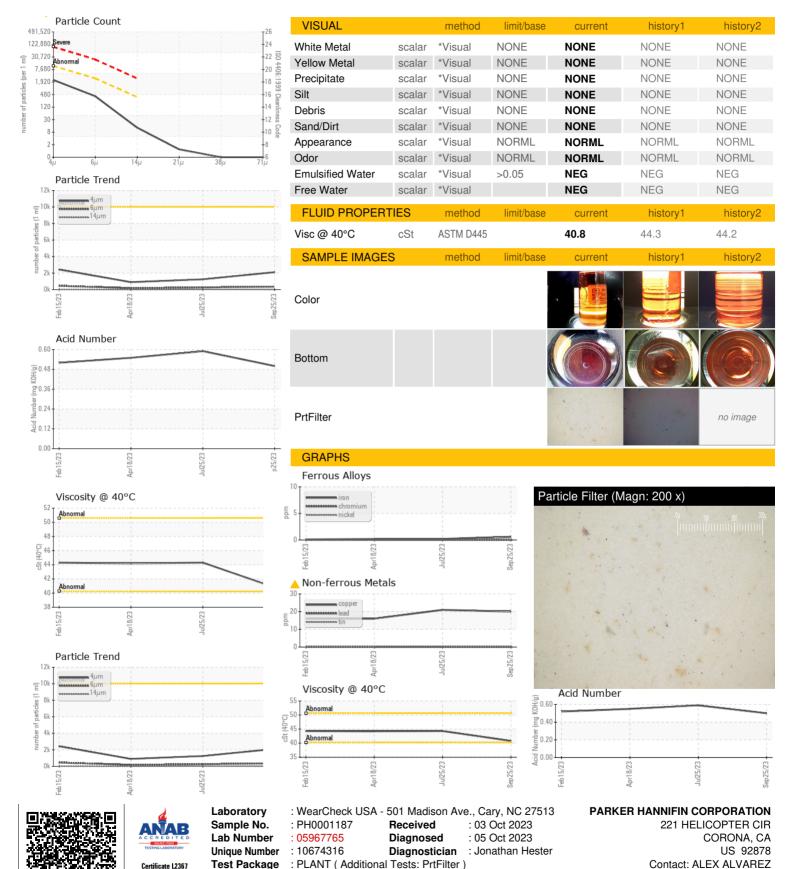

To discuss this sample report, contact Customer Service at 1-800-237-1369.

\* - Denotes test methods that are outside of the ISO 17025 scope of accreditation.

Statements of conformity to specifications are based on the simple acceptance decision rule (JCGM 106:2012)

alex.alvarez@parker.com

T: (951)475-6106