



PROBLEM SUMMARY

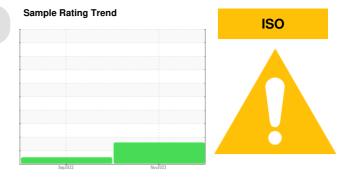

KAESER 7179485

Component Compressor Fluid KAESER SIGMA (OEM) M-460 (--- QTS)

COMPONENT CONDITION SUMMARY

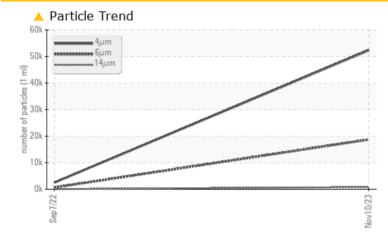

RECOMMENDATION

The filter change at the time of sampling has been noted. Resample at the next service interval to monitor.

PROBLEMATIC TEST	RESULTS				
Sample Status			ABNORMAL	NORMAL	
Particles >6µm	ASTM D7647	>1300	<u> </u>	664	
Particles >14µm	ASTM D7647	>80	<u> </u>	58	
Particles >21µm	ASTM D7647	>20	🔺 116	15	
Oil Cleanliness	ISO 4406 (c)	>/17/13	<u> </u>	19/17/13	

Customer Id: AMABEA Sample No.: KCPA007318 Lab Number: 06016421 Test Package: IND 2



To manage this report scan the QR code

To discuss the diagnosis or test data: Jonathan Hester +1 919-379-4092 x4092 jhester@wearcheckusa.com

To change component or sample information: Customer Service +1 1-800-237-1369 <u>customerservice@wearcheck.com</u> There are no recommended actions for this sample.

HISTORICAL DIAGNOSIS

07 Sep 2022 Diag: Don Baldridge

NORMAL



Resample at the next service interval to monitor.All component wear rates are normal. The amount and size of particulates present in the system are acceptable. There is no indication of any contamination in the oil. The AN level is acceptable for this fluid. The condition of the oil is suitable for further service.





OIL ANALYSIS REPORT

Sample Rating Trend

ISO

KAESER 7179485

Compressor

Fluid KAESER SIGMA (OEM) M-460 (--- QTS)

DIAGNOSIS

Recommendation

The filter change at the time of sampling has been noted. Resample at the next service interval to monitor.

Wear

All component wear rates are normal.

Contamination

There is a high amount of particulates present in the oil.

Fluid Condition


The AN level is acceptable for this fluid. The condition of the oil is suitable for further service.


			Sep2022	Nov2023		
SAMPLE INFORM	MATION	method	limit/base	current	history1	history2
Sample Number		Client Info		KCPA007318	KCP50162	
Sample Date		Client Info		10 Nov 2023	07 Sep 2022	
Machine Age	hrs	Client Info		17370	11341	
Oil Age	hrs	Client Info		0	3000	
Oil Changed		Client Info		N/A	Changed	
Sample Status				ABNORMAL	NORMAL	
WEAR METALS		method	limit/base	current	history1	history2
Iron	ppm	ASTM D5185m	>50	<1	0	
Chromium	ppm	ASTM D5185m	>10	<1	0	
Nickel	ppm	ASTM D5185m	>3	<1	0	
Titanium	ppm	ASTM D5185m		<1	<1	
Silver	ppm	ASTM D5185m	>2	0	0	
Aluminum	ppm	ASTM D5185m		2	0	
Lead		ASTM D5185m	>10	0	0	
	ppm			4	7	
Copper	ppm	ASTM D5185m		-		
Tin	ppm	ASTM D5185m	>10	0	<1	
Vanadium	ppm	ASTM D5185m		0	<1	
Cadmium	ppm	ASTM D5185m		<1	0	
ADDITIVES		method	limit/base	current	history1	history2
Boron	ppm	ASTM D5185m	0	0	0	
Barium	ppm	ASTM D5185m	90	8	0	
Molybdenum	ppm	ASTM D5185m	0	<1	<1	
Manganese	ppm	ASTM D5185m		0	<1	
Magnesium	ppm	ASTM D5185m	100	52	35	
Calcium	ppm	ASTM D5185m	0	1	0	
Phosphorus	ppm	ASTM D5185m	0	0	5	
Zinc	ppm	ASTM D5185m	0	0	0	
Sulfur	ppm	ASTM D5185m	23500	22849	24708	
CONTAMINANTS		method	limit/base	current	history1	history2
Silicon	ppm	ASTM D5185m	>25	1	1	
Sodium	ppm	ASTM D5185m	>25	7	6	
Potassium		ASTM D5185m	>20	3	0	
	ppm			-		
Water Water	%	ASTM D6304		0.022	0.019	
ppm Water	ppm	ASTM D6304	>500	225	193.7	
FLUID CLEANLIN	IESS	method	limit/base	current	history1	history2
Particles >4µm		ASTM D7647		52308	2527	
Particles >6µm		ASTM D7647		<u> </u>	664	
Particles >14µm		ASTM D7647	>80	<u> </u>	58	
Particles >21µm		ASTM D7647	>20	🔺 116	15	
Particles >38µm		ASTM D7647	>4	1	2	
Particles >71µm		ASTM D7647	>3	0	0	
Oil Cleanliness		ISO 4406 (c)	>/17/13	4 23/21/17	19/17/13	
FLUID DEGRADA		method	limit/base	current	history1	history2
Acid Number (AN)	mg KOH/g	ASTM D8045	1.0	0.42	0.41	
	ing NOLLY	AO I M D0040	1.0	0.72	0.71	





Built for a lifetime

OIL ANALYSIS REPORT





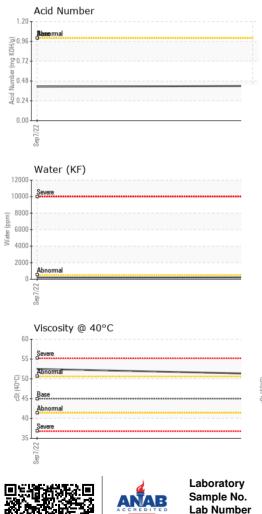

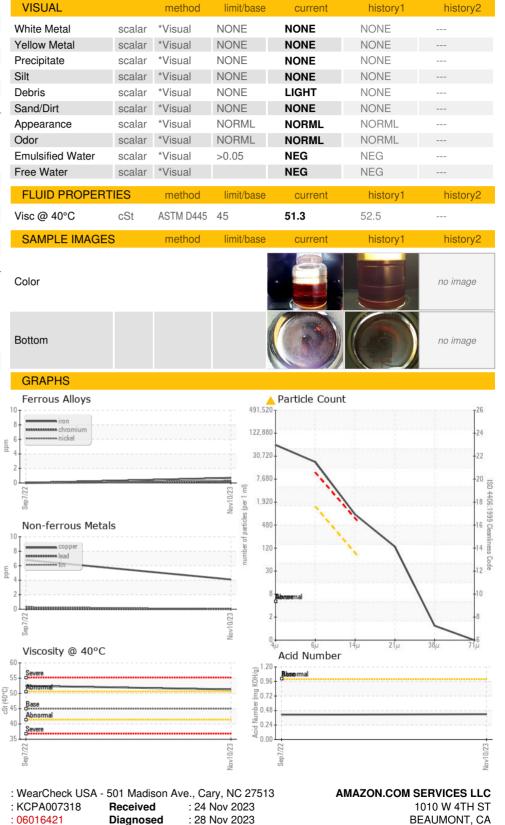

To discuss this sample report, contact Customer Service at 1-800-237-1369. * - Denotes test methods that are outside of the ISO 17025 scope of accreditation.

Test Package : IND 2 (Additional Tests: KF, PrtCount)

: 10755565

Statements of conformity to specifications are based on the simple acceptance decision rule (JCGM 106:2012)

Diagnostician : Jonathan Hester

Certificate L2367

Unique Number

US 92223

T:

F:

Contact: Service Manager