




# OIL ANALYSIS REPORT

Sample Rating Trend

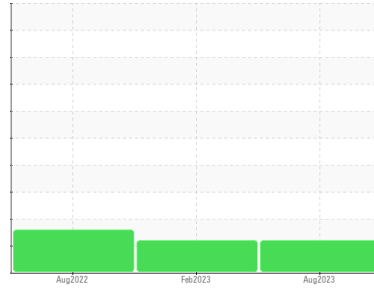

ISO



Machine Id  
**KAESER 7808797 (S/N 1054)**

Component  
**Compressor**

Fluid  
**KAESER SIGMA (OEM) S-460 (--- GAL)**

## DIAGNOSIS

### ▲ Recommendation

No corrective action is recommended at this time. The filter change at the time of sampling has been noted. Resample at the next service interval to monitor.

### Wear

All component wear rates are normal.

### ▲ Contamination

There is a moderate amount of particulates present in the oil.

### Fluid Condition

The AN level is acceptable for this fluid. The condition of the oil is suitable for further service.

SAMPLE INFORMATION		method	limit/base	current	history1	history2
Sample Number	Client Info			<b>KC105971</b>	KC96826	KC103210
Sample Date	Client Info			<b>04 Aug 2023</b>	21 Feb 2023	05 Aug 2022
Machine Age	hrs	Client Info		<b>3375</b>	2956	2442
Oil Age	hrs	Client Info		<b>0</b>	782	268
Oil Changed	Client Info			<b>N/A</b>	Changed	Not Changed
Sample Status				<b>ATTENTION</b>	ABNORMAL	ABNORMAL

WEAR METALS		method	limit/base	current	history1	history2
Iron	ppm	ASTM D5185m	>50	<b>&lt;1</b>	<1	<1
Chromium	ppm	ASTM D5185m	>10	<b>0</b>	0	0
Nickel	ppm	ASTM D5185m	>3	<b>0</b>	0	0
Titanium	ppm	ASTM D5185m	>3	<b>0</b>	0	0
Silver	ppm	ASTM D5185m	>2	<b>0</b>	0	0
Aluminum	ppm	ASTM D5185m	>10	<b>1</b>	<1	<1
Lead	ppm	ASTM D5185m	>10	<b>0</b>	0	<1
Copper	ppm	ASTM D5185m	>50	<b>&lt;1</b>	1	2
Tin	ppm	ASTM D5185m	>10	<b>0</b>	0	<1
Vanadium	ppm	ASTM D5185m		<b>0</b>	0	0
Cadmium	ppm	ASTM D5185m		<b>0</b>	0	0






ADDITIVES		method	limit/base	current	history1	history2
Boron	ppm	ASTM D5185m		<b>0</b>	0	1
Barium	ppm	ASTM D5185m	90	<b>9</b>	<1	<1
Molybdenum	ppm	ASTM D5185m		<b>0</b>	0	0
Manganese	ppm	ASTM D5185m		<b>0</b>	<1	<1
Magnesium	ppm	ASTM D5185m	90	<b>70</b>	56	57
Calcium	ppm	ASTM D5185m	2	<b>2</b>	0	0
Phosphorus	ppm	ASTM D5185m		<b>12</b>	2	7
Zinc	ppm	ASTM D5185m		<b>0</b>	10	14

CONTAMINANTS		method	limit/base	current	history1	history2
Silicon	ppm	ASTM D5185m	>25	<b>&lt;1</b>	<1	<1
Sodium	ppm	ASTM D5185m		<b>15</b>	12	16
Potassium	ppm	ASTM D5185m	>20	<b>2</b>	2	1
Water	%	ASTM D6304	>0.05	<b>0.012</b>	0.008	0.023
ppm Water	ppm	ASTM D6304	>500	<b>130</b>	89.5	238.6

FLUID CLEANLINESS		method	limit/base	current	history1	history2
Particles >4µm		ASTM D7647		<b>4279</b>	4825	6043
Particles >6µm		ASTM D7647	>1300	▲ <b>2372</b>	▲ 2566	▲ 2872
Particles >14µm		ASTM D7647	>80	▲ <b>131</b>	▲ 128	▲ 124
Particles >21µm		ASTM D7647	>20	<b>10</b>	11	▲ 21
Particles >38µm		ASTM D7647	>4	<b>0</b>	0	0
Particles >71µm		ASTM D7647	>3	<b>0</b>	0	0
Oil Cleanliness		ISO 4406 (c)	>--/17/13	▲ <b>19/18/14</b>	▲ 19/19/14	▲ 20/19/14

FLUID DEGRADATION		method	limit/base	current	history1	history2
Acid Number (AN)	mg KOH/g	ASTM D8045	0.4	<b>0.350</b>	0.33	0.35


# OIL ANALYSIS REPORT

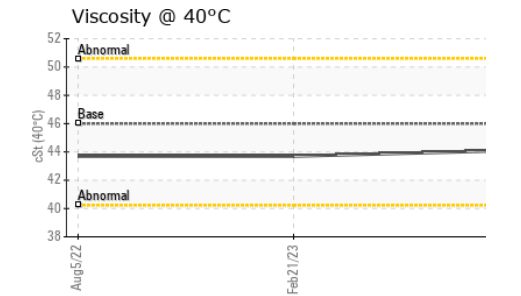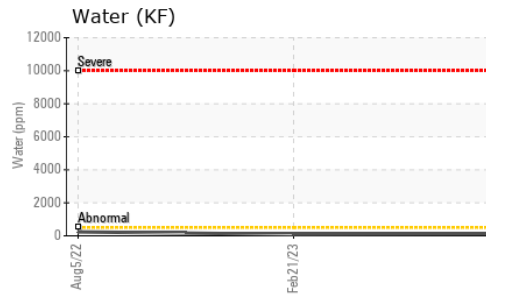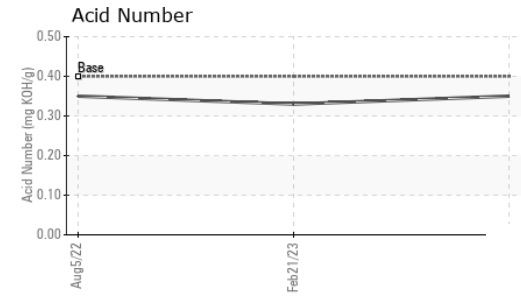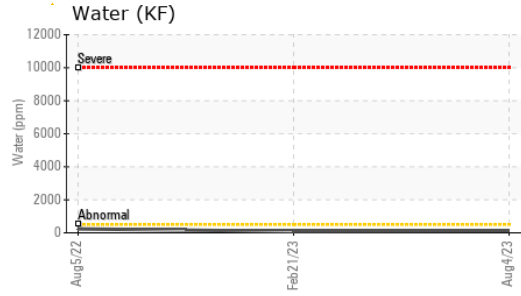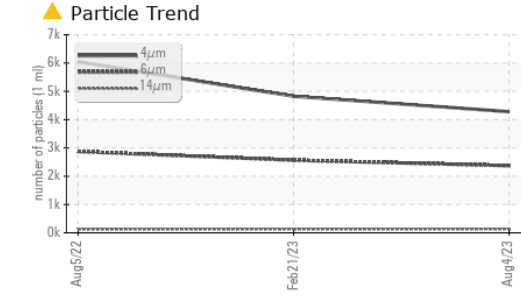





VISUAL	method	limit/base	current	history1	history2
White Metal	scalar	*Visual	NONE	NONE	NONE
Yellow Metal	scalar	*Visual	NONE	NONE	NONE
Precipitate	scalar	*Visual	NONE	NONE	NONE
Silt	scalar	*Visual	NONE	NONE	NONE
Debris	scalar	*Visual	NONE	NONE	NONE
Sand/Dirt	scalar	*Visual	NONE	NONE	NONE
Appearance	scalar	*Visual	NORML	NORML	NORML
Odor	scalar	*Visual	NORML	NORML	NORML
Emulsified Water	scalar	*Visual	>0.05	NEG	NEG
Free Water	scalar	*Visual		NEG	NEG

FLUID PROPERTIES	method	limit/base	current	history1	history2
Visc @ 40°C	cSt	ASTM D445 46	44.1	43.7	43.7

SAMPLE IMAGES	method	limit/base	current	history1	history2
---------------	--------	------------	---------	----------	----------

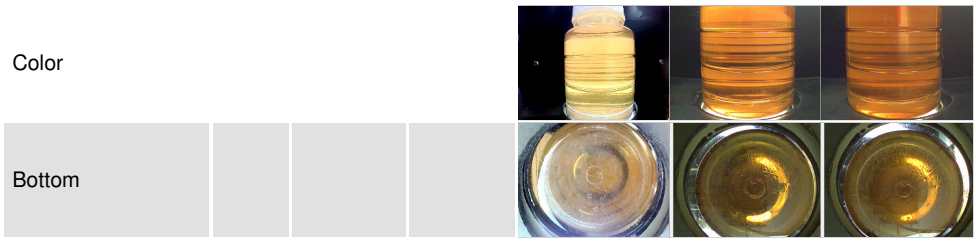

## GRAPHS

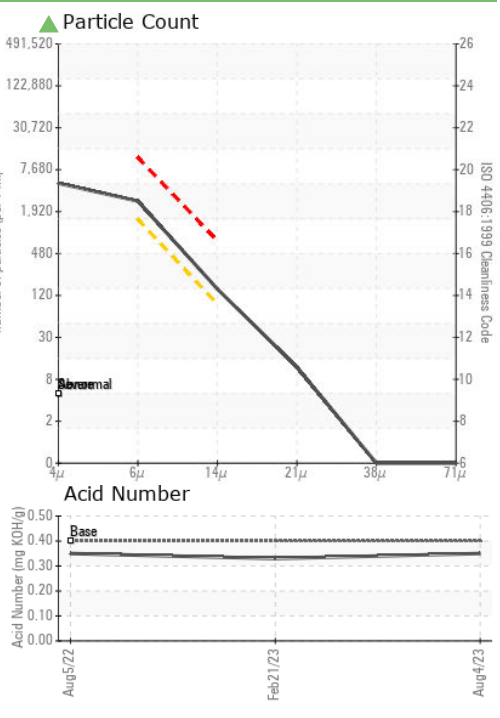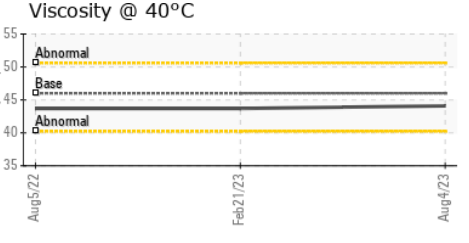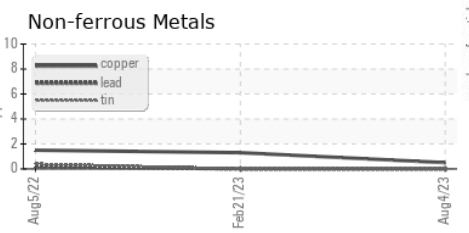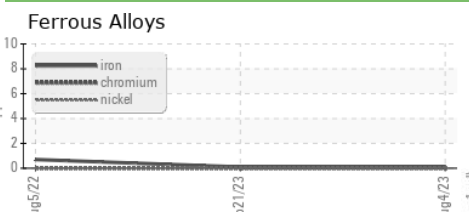

**Laboratory** : WearCheck USA - 501 Madison Ave., Cary, NC 27513  
**Sample No.** : KC105971 **Received** : 16 Jan 2024  
**Lab Number** : 06062016 **Diagnosed** : 18 Jan 2024  
**Unique Number** : 10833398 **Diagnostician** : Don Baldrige  
**Test Package** : IND 2

**ADESA INDIANAPOLIS**  
 2950 E MAIN ST  
 PLAINFIELD, IN  
 US 46168  
 Contact: HECTOR BONET  
 hector.bonet@adesa.com  
 T:  
 F:

To discuss this sample report, contact Customer Service at 1-800-237-1369.  
 \* - Denotes test methods that are outside of the ISO 17025 scope of accreditation.  
 Statements of conformity to specifications are based on the simple acceptance decision rule (JCGM 106:2012)