




# OIL ANALYSIS REPORT

Sample Rating Trend

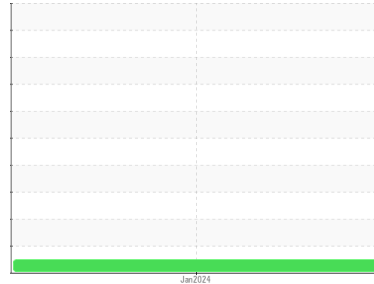

**NORMAL**



Machine Id  
**CAMCO 717 SC**  
 Component  
**New (Unused) Oil**  
 Fluid  
**{not provided} (--- GAL)**

## DIAGNOSIS

### Recommendation

This is a baseline read-out on the submitted sample.

SAMPLE INFORMATION		method	limit/base	current	history1	history2
Sample Number	Client Info			<b>WC0885515</b>	---	---
Sample Date	Client Info			<b>25 Jan 2024</b>	---	---
Machine Age	hrs	Client Info		<b>0</b>	---	---
Oil Age	hrs	Client Info		<b>0</b>	---	---
Oil Changed	Client Info			<b>N/A</b>	---	---
Sample Status				<b>NORMAL</b>	---	---

WEAR METALS		method	limit/base	current	history1	history2
Iron	ppm	ASTM D5185m	>5	<b>0</b>	---	---
Chromium	ppm	ASTM D5185m	>5	<b>0</b>	---	---
Nickel	ppm	ASTM D5185m	>5	<b>0</b>	---	---
Titanium	ppm	ASTM D5185m		<b>&lt;1</b>	---	---
Silver	ppm	ASTM D5185m	>5	<b>0</b>	---	---
Aluminum	ppm	ASTM D5185m	>5	<b>0</b>	---	---
Lead	ppm	ASTM D5185m	>5	<b>0</b>	---	---
Copper	ppm	ASTM D5185m	>5	<b>0</b>	---	---
Tin	ppm	ASTM D5185m	>5	<b>0</b>	---	---
Vanadium	ppm	ASTM D5185m		<b>&lt;1</b>	---	---
Cadmium	ppm	ASTM D5185m		<b>0</b>	---	---

ADDITIVES		method	limit/base	current	history1	history2
Boron	ppm	ASTM D5185m		<b>0</b>	---	---
Barium	ppm	ASTM D5185m		<b>0</b>	---	---
Molybdenum	ppm	ASTM D5185m		<b>0</b>	---	---
Manganese	ppm	ASTM D5185m		<b>&lt;1</b>	---	---
Magnesium	ppm	ASTM D5185m		<b>103</b>	---	---
Calcium	ppm	ASTM D5185m		<b>77</b>	---	---
Phosphorus	ppm	ASTM D5185m		<b>339</b>	---	---
Zinc	ppm	ASTM D5185m		<b>402</b>	---	---
Sulfur	ppm	ASTM D5185m		<b>5688</b>	---	---


CONTAMINANTS		method	limit/base	current	history1	history2
Silicon	ppm	ASTM D5185m	>15	<b>&lt;1</b>	---	---
Sodium	ppm	ASTM D5185m		<b>2</b>	---	---
Potassium	ppm	ASTM D5185m	>20	<b>0</b>	---	---
Water	%	ASTM D6304		<b>0.002</b>	---	---
ppm Water	ppm	ASTM D6304		<b>24</b>	---	---

FLUID CLEANLINESS		method	limit/base	current	history1	history2
Particles >4µm		ASTM D7647	>5000	<b>1304</b>	---	---
Particles >6µm		ASTM D7647	>1300	<b>281</b>	---	---
Particles >14µm		ASTM D7647	>160	<b>23</b>	---	---
Particles >21µm		ASTM D7647	>40	<b>7</b>	---	---
Particles >38µm		ASTM D7647	>10	<b>0</b>	---	---
Particles >71µm		ASTM D7647	>3	<b>0</b>	---	---
Oil Cleanliness		ISO 4406 (c)	>19/17/14	<b>18/15/12</b>	---	---


FLUID DEGRADATION		method	limit/base	current	history1	history2
Acid Number (AN)	mg KOH/g	ASTM D8045		<b>0.046</b>	---	---




# OIL ANALYSIS REPORT

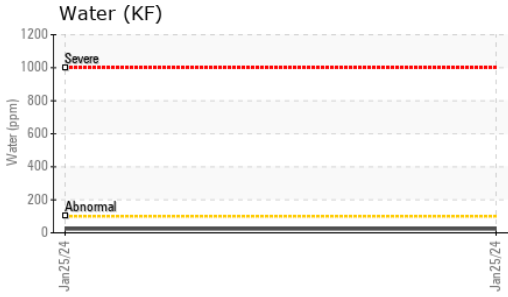

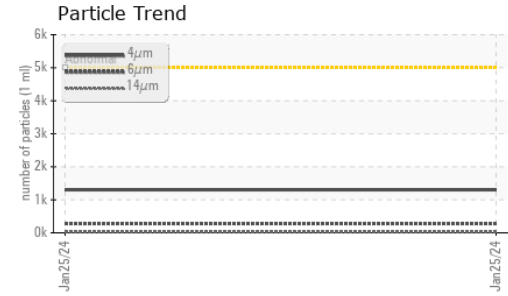


VISUAL	method	limit/base	current	history1	history2
White Metal	scalar	*Visual	NONE	NONE	---
Yellow Metal	scalar	*Visual	NONE	NONE	---
Precipitate	scalar	*Visual	NONE	NONE	---
Silt	scalar	*Visual	NONE	NONE	---
Debris	scalar	*Visual	NONE	NONE	---
Sand/Dirt	scalar	*Visual	NONE	NONE	---
Appearance	scalar	*Visual	NORML	NORML	---
Odor	scalar	*Visual	NORML	NORML	---
Emulsified Water	scalar	*Visual	NEG	---	---
Free Water	scalar	*Visual	NEG	---	---

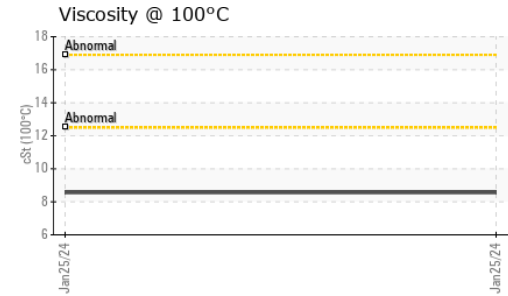







FLUID PROPERTIES	method	limit/base	current	history1	history2
Visc @ 40°C	cSt	ASTM D445	63.71	---	---
Visc @ 100°C	cSt	ASTM D445	8.56	---	---
Viscosity Index (VI)	Scale	ASTM D2270	105	---	---



SAMPLE IMAGES	method	limit/base	current	history1	history2
Color				no image	no image
Bottom				no image	no image

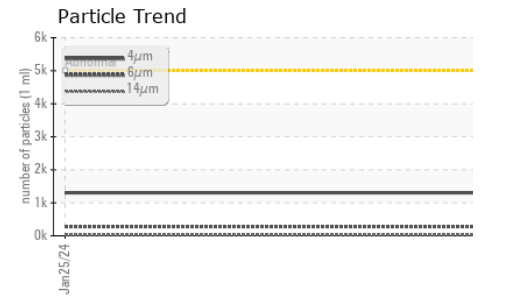

## GRAPHS

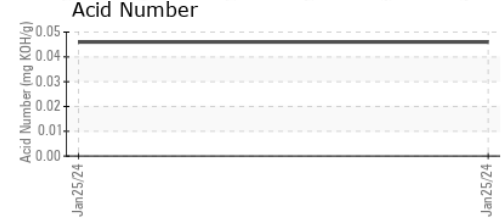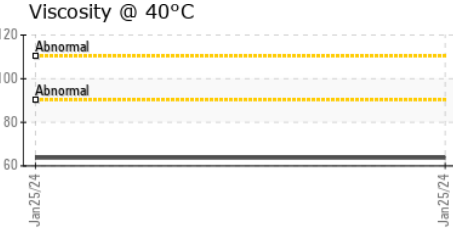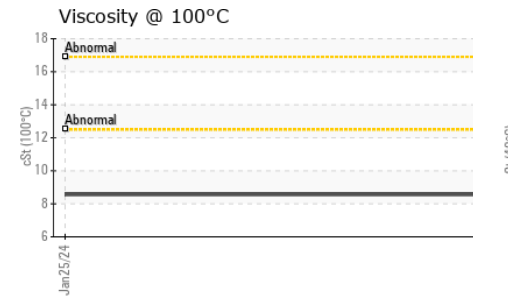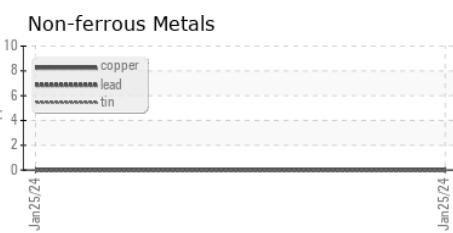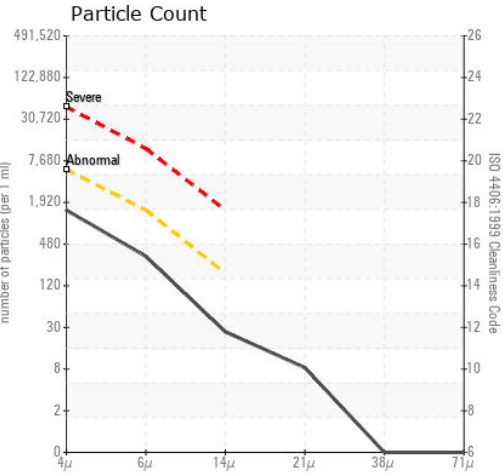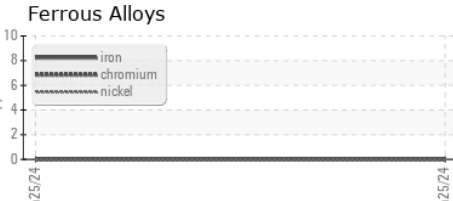

**Laboratory** : WearCheck USA - 501 Madison Ave., Cary, NC 27513  
**Sample No.** : WC0885515 **Received** : 30 Jan 2024  
**Lab Number** : 06075278 **Diagnosed** : 05 Feb 2024  
**Unique Number** : 10857369 **Diagnostician** : Jonathan Hester  
**Test Package** : IND 2 ( Additional Tests: FT-IR, ICP-NewOil, KF, KV100, PrtCount, VI )

**LLOYDS BARBEQUE COMPANY - HORMEL**  
 1455 MENDOTA HEIGHTS RD  
 SAINT PAUL, MN  
 US 55120  
 Contact: PAT HUMPHREY  
 PAHumphrey@Hormel.com  
 T: (651)905-8767  
 F: (651)688-6000

Certificate L2367  
 To discuss this sample report, contact Customer Service at 1-800-237-1369.  
 \* - Denotes test methods that are outside of the ISO 17025 scope of accreditation.  
 Statements of conformity to specifications are based on the simple acceptance decision rule (JCGM 106:2012)