

OIL ANALYSIS REPORT

Area BEACON MEDAES VAC PUMP [153303] Machine Id BEACON MEDAES DEM119230532 - AURORA Component

Compressor

DIAGNOSIS

Recommendation

Resample at the next service interval to monitor.

Wear


All component wear rates are normal.

Contamination

There is no indication of any contamination in the oil.

Fluid Condition

The AN level is acceptable for this fluid. The condition of the oil is suitable for further service.






NORMAL

SAMPLE INFORM	/IATION	method	limit/base	current	history1	history2
Sample Number		Client Info		UCH06122502		
Sample Date		Client Info		14 Mar 2024		
Machine Age	hrs	Client Info		9284		
Oil Age	hrs	Client Info		2207		
Oil Changed		Client Info		Changed		
Sample Status				NORMAL		
CONTAMINATIO	N	method	limit/base	current	history1	history2
Water		WC Method	>0.1	NEG		
WEAR METALS		method	limit/base	current	history1	history2
Iron	ppm	ASTM D5185m	>50	0		
Chromium	ppm	ASTM D5185m	>10	0		
Nickel	ppm	ASTM D5185m		0		
Titanium	ppm	ASTM D5185m		0		
Silver	ppm	ASTM D5185m		0		
Aluminum	ppm	ASTM D5185m	>25	0		
Lead	ppm	ASTM D5185m	>25	0		
Copper	ppm	ASTM D5185m	>50	0		
Tin	ppm	ASTM D5185m	>15	0		
Vanadium	ppm	ASTM D5185m		0		
Cadmium	ppm	ASTM D5185m		0		
ADDITIVES		method	limit/base	current	history1	history2
Boron	ppm	ASTM D5185m	150	0		
Barium	ppm	ASTM D5185m		0		
Molybdenum	ppm	ASTM D5185m		0		
Manganese	ppm	ASTM D5185m		0		
Magnesium	ppm	ASTM D5185m	10	0		
Calcium	ppm	ASTM D5185m	70	0		
Phosphorus	ppm	ASTM D5185m	2000	1657		
Zinc	ppm	ASTM D5185m	50	0		
Sulfur	ppm	ASTM D5185m	20000	1028		
CONTAMINANTS	;	method	limit/base	current	history1	history2
Silicon	ppm	ASTM D5185m	>25	0		
Sodium	ppm	ASTM D5185m		0		
Potassium	ppm	ASTM D5185m	>20	0		
FLUID DEGRADA	TION	method	limit/base	current	history1	history2
Acid Number (AN)	mg KOH/g	ASTM D8045		0.077		



Marl

OIL ANALYSIS REPORT

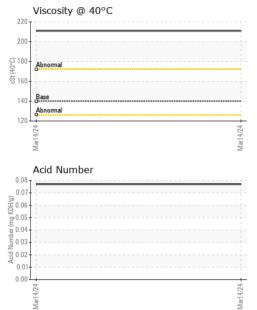

	VISUAL		method	limit/base	current	history1	history2
	White Metal	scalar	*Visual	NONE	NONE		
	Yellow Metal	scalar	*Visual	NONE	NONE		
	Precipitate	scalar	*Visual	NONE	NONE		
	Silt	scalar	*Visual	NONE	NONE		
	Debris	scalar	*Visual	NONE	NONE		
	Sand/Dirt	scalar	*Visual	NONE	NONE		
4/24 -	Appearance	scalar	*Visual	NORML	NORML		
Mar14/24	Odor	scalar	*Visual	NORML	NORML		
	Emulsified Water	scalar	*Visual	>0.1	NEG		
	Free Water	scalar	*Visual		NEG		
				1:		la la tamurt	history.O
	FLUID PROPER		method	limit/base	current	history1	history2
	Visc @ 40°C	cSt	ASTM D445	140	211		
	SAMPLE IMAGE	S	method	limit/base	current	history1	history2
Mar14/24	Color					no image	no image
	Bottom					no image	no image
	Non-ferrous Meta	ls		Mari 4/24 Mari 4/24			
	Viscosity @ 40°C			Mar1 4/24	Acid Number		
	: WearCheck USA - 50 : UCH06122502 : 06122502 : 10936653 : IND 2 ; contact Customer Serv	Recei Teste Diagr	ison Ave., Cary, NC 27513 ceived : 19 Mar 2024 sted : 20 Mar 2024 ignosed : 21 Mar 2024 - Sean Felton			BEACON MEDAE 1059 PARAGON WA ROCKHILL, S US 2973 Contact: ED L ed.lou@beaconmedaes.co T 6:2012) F: (803)817-578	

Statements of conformity to specifications are based on the simple acceptance decision rule (JCGM 106:2012) F: (803)817-5788

Contact/Location: ED LU - UCBEAROC